

Preprocessing: A Step in Automating Early Detection of Cervical Cancer

Abhishek Das ^a, Avijit Kar ^a and Debasis Bhattacharyya ^b

^a*Dept. of Computer Sc. & Engineering, Jadavpur University
Kolkata, India*

^b*Dept. of Gynecology & Obstetrics, SSKM Hospital
Kolkata, India*

Abstract. Uterine Cervical Cancer is one of the most common forms of cancer in women worldwide. Most cases of cervical cancer can be prevented through screening programs aimed at detecting precancerous lesions. During Digital Colposcopy, colposcopic images or cervigrams are acquired in raw form. They contain specular reflections which appear as bright spots heavily saturated with white light and occur due to the presence of moisture on the uneven cervix surface and. The cervix region occupies about half of the raw cervigram image. Other parts of the image contain irrelevant information, such as equipment, frames, text and non-cervix tissues. This irrelevant information can confuse automatic identification of the tissues within the cervix. Therefore we focus on the cervical borders, so that we have a geometric boundary on the relevant image area. Our novel technique eliminates the SR, identifies the region of interest and makes the cervigram ready for segmentation algorithms.

Keywords. cervix; region of interest; preprocessing; segmentation; clustering

Introduction

Cervical Cancer is one of the most common forms of cancer in woman worldwide. Colposcopy is an effective diagnostic tool where the cervix is examined non-invasively by a specially designed microscope(colposcope). The abnormal cervical regions turn to be white after application of 5% acetic acid and are called Acetowhite(AW) lesions which are then biopsied under colposcopic guidance for confirmation by histopathological examination. Digital Colposcope produces a digital image of the cervix and is considered the *gold standard* for detection and treatment of pre-cancerous lesions of the cervix or Cervical Intra-epithelial Neoplasia(CIN). However, there is currently a void in specialized image processing software which has the ability to process images acquired in colposcopy. The purpose of the paper is to present image processing methods to make the cervigram ready for segmentation algorithms.

1. Automated System

An automated system is proposed in this paper that is used for diagnosis of CIN. The scheme is presented as a block diagram in Fig. 1. The process of translating raw cervix image acquired using a Digital Colposcope into a thorough diagnosis of CIN is decomposed into four modules as shown in Fig. 1. However, we are presenting the first two modules in this paper.

1.1. Removal of Specular Reflection

Specular reflections (SR) appear as bright spots heavily saturated with white light and occur due to the presence of moisture on the uneven cervix surface. At first, the RGB Image (raw Cervigram) is separated to the Red, Green and Blue Planes. Standard Morphological methods are used that utilize a structuring element (SE). Once the dilated binary images with outlines are identified, the borders of all the reflections on the original grayscale image using the coordinates are returned. A filling algorithm is used which smoothly interpolates inward from the pixel values on the boundary of the polygon (white SR areas) by solving Laplace's equation.

1.2. Cervix ROI Segmentation

The cervix region involves about half of the cervigram image. Other parts of the image contain irrelevant information, such as equipment, frames, text, and non-cervix tissues. This irrelevant information can confuse the automatic identification of the tissues within the cervix. A Modified K-means Clustering Algorithm is used to get the ROI.


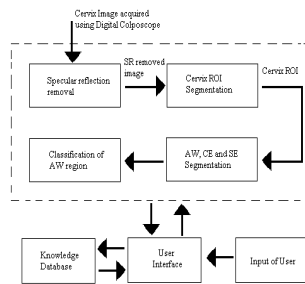


Fig1: Block Diagram of the proposed Automation tool for CIN detection

Fig2: Raw Cervigram (left), Specular reflection removed image (centre), ROI detected using clustering algorithm (right)

Conclusion

We have used a dataset of 100 Normal cervigrams and 25 Acetowhite cervigrams. On visual inspection by Gyneco-oncologists of previous research results [1]-[3], our method of removal of specular reflection is far better, as it smoothly interpolates using our algorithm.

References

- [1] P. M. Cristoforoni, D. Gerbaldo, F. J. Montz, and G. L. Capitanio, "Computerized colposcopy: results of a pilot study and analysis of its clinical relevance," *Obstet. Gynecol.* 85(1995), 1011-1016.
- [2] W. Li, V. Van Raad, , and D. Ferris, "Computer-aided diagnosis (CAD)for cervical cancer screening and diagnosis: a new system design in medical image processing," *LNCS*, 3765(2005), 240-250 .
- [3] S. Gordon, G. Zimmerman, and H.Greenspan, "Content analysis of uterine cervix images: Initial steps towards content based indexing and retrieval of cervigrams," *Proc. SPIE Conf. on Medical Imaging*, 6144(2006), 1549-1556.