

Medical Image Analysis of Brain X-ray CT Images By Deep GMDH-Type Neural Network

Tadashi Kondo[†]

*Graduate School of Health Sciences, Tokushima University
3-18-15 Kuramoto-cho Tokushima 770-8509 Japan
Email: [†]kondomedsci@gmail.com*

Junji Ueno

*Graduate School of Health Sciences, Tokushima University
3-18-15 Kuramoto-cho Tokushima 770-8509 Japan*

Shoichiro Takao

*Graduate School of Health Sciences, Tokushima University
3-18-15 Kuramoto-cho Tokushima 770-8509 Japan*

Abstract

The deep Group Method of Data Handling (GMDH)-type neural network is applied to the medical image analysis of brain X-ray CT image. In this algorithm, the deep neural network architectures which have many hidden layers and fit the complexity of the nonlinear systems, are automatically organized using the heuristic self-organization method so as to minimize the prediction error criterion defined as Akaike's Information Criterion (AIC) or Prediction Sum of Squares (PSS). The learning algorithm is the principal component-regression analysis and the accurate and stable predicted values are obtained. The recognition results show that the deep GMDH-type neural network algorithm is useful for the medical image analysis of brain X-ray CT images.

Keywords: Deep neural networks, GMDH, Medical image recognition, Evolutionary computation, X-ray CT image.

1. Introduction

The deep GMDH-type neural network algorithms were proposed in our early works¹⁻⁴ and can automatically organize the neural network architectures using heuristic self-organization method^{5,6} which is a type of the evolutionary computation. In this study, deep GMDH-type neural network algorithm¹ is applied to the medical image analysis of brain X-ray CT images. The learning calculations of the weights is the principal component-regression analysis and the accurate and stable predicted values are obtained. In this GMDH-type neural network, two types of neurons such as the sigmoid function neuron and the polynomial neuron are used to organize the deep neural network and very complex nonlinear systems can be identified using this deep GMDH-type neural network. In our previous

work², we have applied the deep multilayered GMDH-type neural network to the medical image recognition of brain and blood vessels. This deep multi-layered GMDH-type neural network selected the sigmoid function neural network architectures from the three types of neural network architectures such as the sigmoid function neural network, the radial basis function (RBF) neural network and the polynomial neural network architecture. The brain and blood vessel regions are recognized and extracted accurately using the sigmoid function neural network architectures. In this study, the deep logistic GMDH-type neural network algorithm is applied to the medical image analysis of brain X-ray CT images and the skull and the blood vessel regions in the brain are recognized and extracted. The recognition results are compared with those obtained using the conventional neural networks trained

using the back propagation algorithm and it is shown that this deep neural network is accurate and useful for the medical image analysis of the brain X-ray CT image.

2. Deep GMDH-type neural network¹

The GMDH-type neural network architecture is shown in Fig.1. Here, nonlinear function g_i is described by the following Kolmogorov-Gabor polynomial:

$$g_i(x_1, x_2, \dots, x_p) = a_0 + \sum_i a_i x_i + \sum_{i,j} a_{ij} x_i x_j + \dots \quad (1)$$

This nonlinear function is automatically organized by using the polynomial neurons. The architecture of the GMDH-type neural network is automatically organized using the heuristic self-organization and is produced as follows:

In the GMDH-type neural network, the original data are not separated into training and test sets because AIC⁷ or PSS⁸ can be used as the test errors.

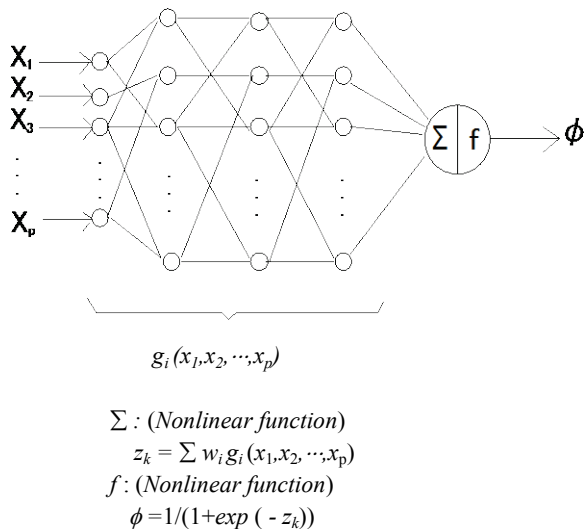


Fig.1 Architecture of the deep GMDH-type neural network

2.1 The first layer

$$u_j = x_j \quad (j=1, 2, \dots, p) \quad (2)$$

where x_j ($j=1, 2, \dots, p$) are the input variables of the system, and p is the number of input variables.

2.2 The second layer

All combinations of two variables (u_i, u_j) are generated. For each combination, the neuron architecture is described by the following equations:

Σ : (Nonlinear function)

$$z_k = w_1 u_i + w_2 u_j + w_3 u_i u_j + w_4 u_i^2 + w_5 u_j^2 - w_0 \theta_l \quad (3)$$

f : (Linear function)

$$y_k = z_k \quad (4)$$

where $\theta_l = 1$ and w_i ($i=0, 1, 2, \dots, 5$) are weights between the first and second layer. The weights w_i ($i=0, 1, 2, \dots, 5$) are estimated by using the principal component-regression analysis. This procedure is as follows:

First, the values of z_k are calculated using the following equation:

$$z_k = \log_e(\phi' / (1 - \phi')) \quad (5)$$

where ϕ' is the normalized output variable. Then the weights w_i ($i=0, 1, 2, \dots, 5$) are estimated by using the principal component-regression analysis.

[Principal component-regression analysis]

In the GMDH-type neural network, the multicollinearity is generated in the function Σ of the neurons because heuristic self-organization method is used. In this study, the function Σ is calculated using the principal component-regression analysis.

In the case of Eq.(3), orthogonal vector \underline{v} is calculated .

$$\underline{v} = C \cdot \underline{u} \quad (6)$$

Here,

$$\underline{v} = (v_1, v_2, \dots, v_5)$$

$$\underline{u} = (u_i, u_j, u_i u_j, u_i^2, u_j^2)$$

\underline{v} is orthonormal vectors and C is orthonormal matrix. C is calculated using the following eigenvalue equation.

$$R \cdot C = C \cdot \Lambda \quad (7)$$

Here, R is a correlation matrix. Then, variable z_k is calculated using orthogonal regression analysis.

$$z_k = \underline{w}^T \cdot \underline{v}$$

$$= w_1 v_1 + w_2 v_2 + \dots + w_5 v_5 \quad (8)$$

Using the principal component-regression analysis, variable z_k in the function Σ is calculated without multicollinearity. In (8), useful orthogonal variables v_i ($i=1, 2, \dots, 5$) are selected by stepwise regression analysis⁹ using AIC or PSS criterion.

From these generated neurons, L neurons which minimize AIC⁷ or PSS⁸ values are selected. The output values (y_k) of L selected neurons are set to the input values of the neurons in the third layer.

2.3 The third and succeeding layers

In the third and succeeding layers, the same computation of the second layer is iterated until AIC or

PSS values of L neurons are not decreased. When the iterative computation is terminated, the following calculation of the output layer is carried out.

2.4 The output layer

In the output layer, the output values of the neural network are calculated from z_k as follows:

$$y_k = 1/(1+exp(-z_k)) \tag{9}$$

So, in the output layer, the neuron architecture becomes as follows:

Σ : (Nonlinear function)

$$z_k = \sum w_i g_i(x_1, x_2, \dots, x_p) \tag{10}$$

f : (Nonlinear function)

$$\phi = 1/(1+exp(-z_k)) \tag{11}$$

The complete neural network architecture is produced by selected neurons in each layer.

In this algorithm, the principal component-regression analysis is used for the learning calculation of the neural network and the accurate and stable prediction values are obtained. The structural parameters such as the number of layers, the number of neurons in hidden layers and useful input variables are automatically selected to minimize prediction error criterion defined as AIC or PSS. The GMDH-type neural network is organized with two types of neurons which are the sigmoid function neuron and the polynomial neuron and this neural network can identify very complex nonlinear system.

3. Application to the medical image analysis of brain X-ray CT images.

In this study, the regions of the skull and the blood vessels in the brain were recognized and extracted automatically. Multi-detector row CT (MDCT) images of the brain are used in this study.

3.1 Extraction of the skull regions

An brain MDCT image shown in Fig.2 was used for organizing the deep GMDH-type neural network. The statistics of the image densities and x and y coordinates in the neighboring regions, the $N \times N$ pixel regions, were used as the image features. The neural networks were organized when the values of N were from 3 to 10. When N was equal to 3, the neural network architecture had the smallest recognition error. Fig.3 shows the

variation of PSS values in each layer. The PSS values were decreased gradually through the layers and small PSS value was obtained in the seventh layer. The deep GMDH-type neural network output the skull image (Fig.4) and the post-processing analysis of the output skull image was carried out. Fig.5 shows the output image after the post-processing. The output image after the post-processing was overlapped to the original image (Fig.2) as shown in Fig.6. The recognized skull region are very accurate. The skull region was extracted from the original image as shown in Fig.7. These image processing were carried out for all slices by the organized deep GMDH-type neural network and the 3-dimensional skull image was generated as shown in Fig.8. A conventional neural network trained using the back propagation algorithm was applied to the same recognition problem. The output images, when the numbers of neurons in the hidden layer (m) are 5, 7 and 9, are shown in Fig.9. These images contain more regions which are not part of the skull.

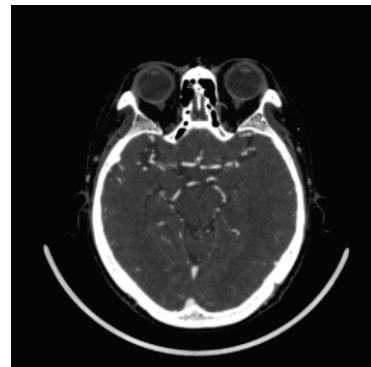


Fig. 2 Original image of the brain

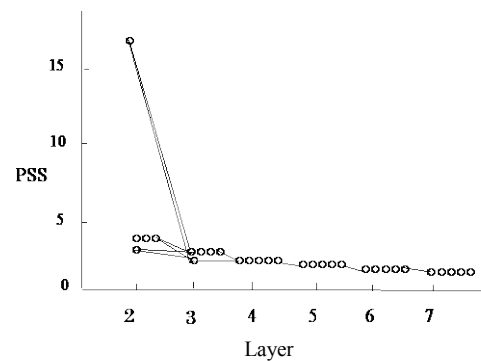


Fig. 3 Variation of PSS values in each layer (1)



Fig. 4 Output image (1)

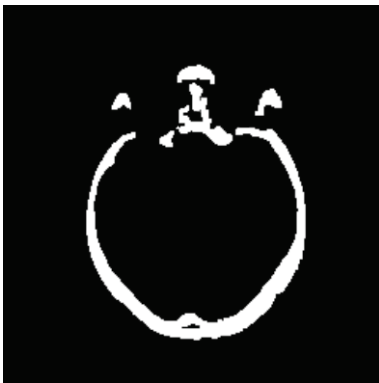


Fig. 5 Output image after the post processing (1)

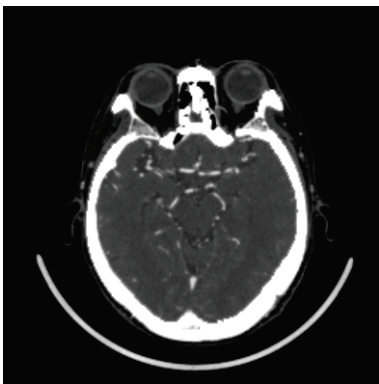


Fig. 6 Overlapped image (1)



Fig. 7 Extracted gray scale image (1) of the skull


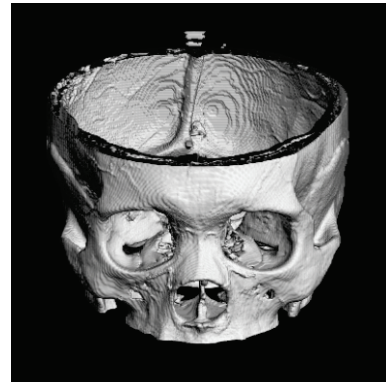



Fig. 8 The 3-dimensional skull image



(a) $m=5$

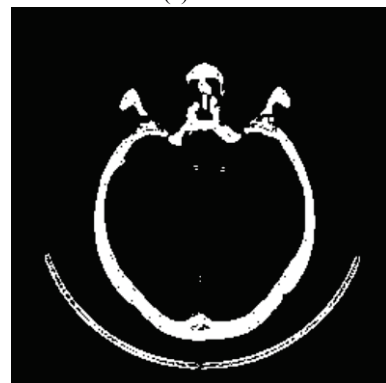

(b) $m=7$

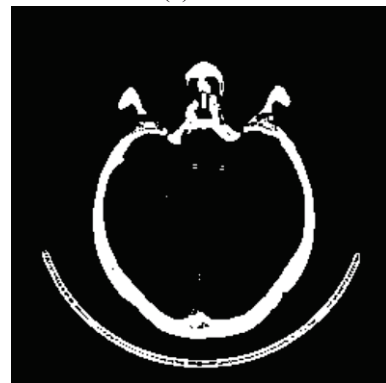

(c) $m=9$

Fig. 9 Output images of the conventional neural network (1)

3.2 Extraction of the blood vessel regions

Another deep GMDH-type neural network was organized and applied to the recognition of the blood vessel regions in the brain using the MDCT image shown in Fig.10 which was extracted from the original image in Fig.2. Fig.11 shows the variation of PSS values in each layer. Very small PSS values were obtained in the seventh layer. The deep GMDH-type neural network output the blood vessel image as shown in Fig.12. The output image after the post-processing (Fig.13) was overlapped as shown in Fig.14. The recognized blood vessel regions were very accurate. The blood vessel regions were extracted from the original image as shown in Fig.15. These image processing were carried out for all slices by the organized deep GMDH-type neural network and the 3-dimensional blood vessel image was generated as shown in Fig.16. A conventional neural network trained using the back propagation algorithm was applied and the output images, when the numbers of neurons in the hidden layer (m) are 5, 7 and 9, are shown in Fig.17. These images contained many noise compared with the output image of the deep GMDH-type neural network which is shown in Fig.12.

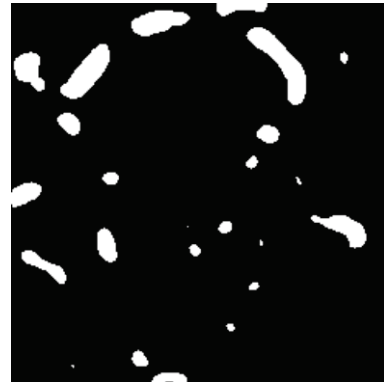


Fig.12 Output image (2)



Fig.13 Output image after the post-processing (2)

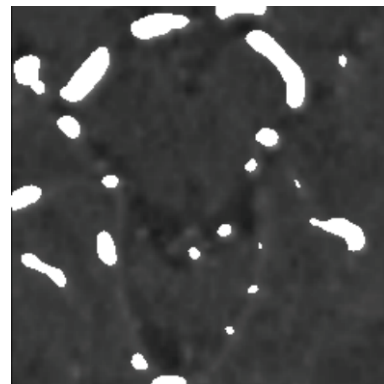


Fig.14 Overlapped image (2)

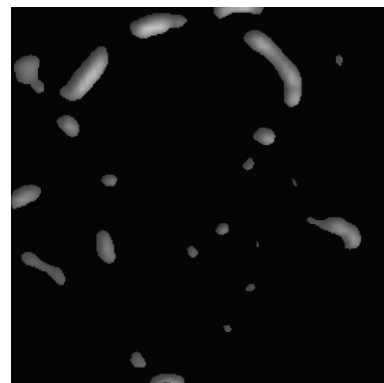


Fig.15 Extracted gray scale image (2) of blood vessels

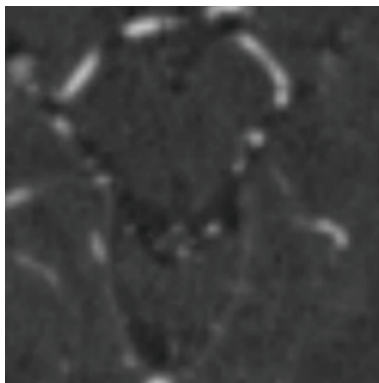


Fig.10 Original image of blood vessels extracted from Fig.2

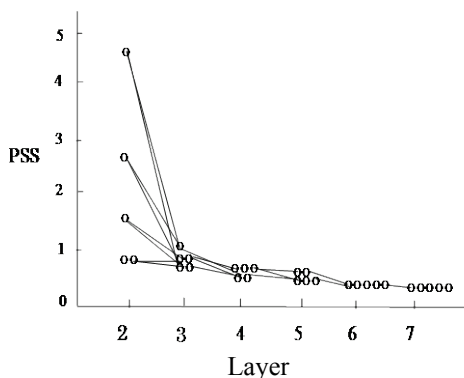


Fig.11 Variation of PSS values in each layer (2)

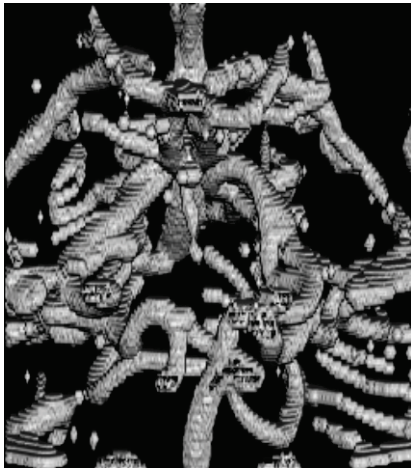


Fig.16 The 3-dimensional blood vessel image

4. Conclusions

In this paper, the deep GMDH-type neural network algorithm using principal component-regression analysis was applied to the medical image analysis of the brain X-ray CT image, and the skull and the blood vessel regions in the brain were recognized and extracted accurately. The deep neural network architectures which had six hidden layers were organized for both skull and blood vessel regions so as to minimize the prediction error criterion defined as PSS. PSS values were gradually decreased through the hidden layers and these PSS values converged on very small PSS value in the seventh layer. The recognition results were compared with those obtained using the conventional neural networks trained using the back propagation algorithm and it was shown that this deep neural networks with many hidden layers were accurate and useful for the medical image analysis of the brain X-ray CT image.

Acknowledgment

This work was supported by (JSPS) KAKENHI 26420421.



(a) $m=5$



(b) $m=7$



(c) $m=9$

Fig.17 Output images of the conventional neural network (2)

References

1. T. Kondo, J. Ueno and S. Takao, Logistic GMDH-type neural network using principal component-regression analysis and its application to medical image diagnosis of lung cancer, *Artificial Life and Robotics* **20**(2)(2015) 137-144.
2. T. Kondo, J. Ueno and S. Takao, Deep multi-layered GMDH-type neural network using principal component-regression analysis and its application to medical image recognition of brain and blood vessels, *Proceedings of the twentieth international symposium on artificial life and robotics* (2015) pp.92-95.
3. T. Kondo, J. Ueno and S. Takao, Medical image recognition of heart regions by deep multi-layered GMDH-type neural network using principal component-regression analysis, *Journal of Robotics, Networking and Artificial Life*, **2**(3)(2015) 166-172.
4. T. Kondo, J. Ueno and S. Takao, Deep feedback GMDH-type neural network using principal component-regression analysis and its application to medical image recognition of abdominal multi-organs, *Journal of Robotics, Networking and Artificial Life* **2**(2)(2015) 94-99.
5. A. G. Ivakhnenko, Heuristic self-organization in problems of engineering cybernetics, *Automatica* **6**(2)(1970) 207-219.
6. S. J. Farlow ed., *Self-organizing methods in modeling, GMDH-type algorithm*, New York: Marcel Dekker Inc., 1984.
7. H. Akaike, A new look at the statistical model identification, *IEEE Trans. Automatic Control*, **AC-19**, (6) (1974) 716-723.
8. H. Tamura, T. Kondo, Heuristics free group method of data handling algorithm of generating optimum partial polynomials with application to air pollution prediction, *Int. J. System Sci.* **11** (9) (1980) 1095-1111.
9. N. R. Draper and H. Smith, *Applied Regression Analysis*, New York: John Wiley and Sons, 1982.