

# Fast & Furious focal-plane wavefront sensing

Visa Korkiakoski,<sup>1,2</sup> Christoph U. Keller,<sup>2</sup> Niek Doelman,<sup>3,2</sup>  
Matthew Kenworthy,<sup>2</sup> Gilles Otten,<sup>2</sup> and Michel Verhaegen<sup>1</sup>

<sup>1</sup>*Delft Center for Systems and Control, Mekelweg 2, 2628CD Delft, The Netherlands\**

<sup>2</sup>*Leiden Observatory, Leiden University, P.O. Box 9513, 2300 RA Leiden, The Netherlands*

<sup>3</sup>*TNO Science and Industry, Stieltjesweg 1, 2628CK Delft, The Netherlands*

compiled: June 5, 2014

We present two complementary algorithms suitable for using focal-plane measurements to control a wavefront corrector with an extremely high spatial resolution. The algorithms use linear approximations to iteratively minimize the aberrations seen by the focal-plane camera. The first algorithm, Fast & Furious (FF), uses a weak-aberration assumption and pupil symmetries to achieve fast wavefront reconstruction. The second algorithm, an extension to FF, can deal with an arbitrary pupil shape; it uses a Gerchberg-Saxton style error reduction to determine the pupil amplitudes. Simulations and experimental results are shown for a spatial light modulator controlling the wavefront with a resolution of  $170 \times 170$  pixels. The algorithms increase the Strehl ratio from  $\sim 0.75$  to  $0.98$ – $0.99$ , and the intensity of the scattered light is reduced throughout the whole recorded image of  $320 \times 320$  pixels. The remaining wavefront rms error is estimated to be  $\sim 0.15$  rad with FF and  $\sim 0.10$  rad with FF-GS.

## 1. Introduction

When an object is imaged, variations of the refractive index in the medium, as well as optical alignment and manufacturing errors, distort the recorded image. This problem is typically solved using active or adaptive optics, where a deformable mirror, spatial light modulator (SLM) or a comparable device corrects the propagating wavefront. Typically, such systems are built with a separate optical arm to measure the distorted wavefront, because extracting the wavefront information from only focal-plane images is not trivial. However, focal-plane wavefront sensing is an active topic – not only to simplify the optical design but also to eliminate the non-common path aberrations limiting the performance of high-contrast adaptive optics systems.

The most popular method for the focal-plane wavefront sensing is perhaps the Gerchberg-Saxton (GS) error reduction algorithm [1, 2] and their variations, for instance [3, 4]. These are numerically very efficient algorithms, and it is easy to modify them for different applications. However, they suffer from accuracy, in particular because their iterative improvement procedure often stagnates at a local minimum.

Various alternatives have been proposed, and a popular approach is to use general numerical optimization techniques to minimize an error function; examples include [5–7]. However, when the number of optimization parameters is increased, the computational requirements generally rise unacceptably fast. The high computational costs are problematic for instance in astronomy; the largest future adaptive optics system is envisioned to have a wavefront corrector of a size of  $200 \times 200$  [8].

The numerical issues can be significantly reduced, if the unknown wavefront is sufficiently small. This is the case, for example, when calibrating the non-common path aberrations. Previous works have exploited the small-phase approximations [9–12], but the implementations are generally not easily extended to the wavefront correction at extremely large resolution, such as over  $100 \times 100$  elements.

In this paper, we present two algorithms capable of extremely fast control of a wavefront correcting device with 20 000–30 000 degrees of freedom.

The first algorithm, Fast & Furious (FF), has been published before [13–15]. It relies on small WF aberrations, pupil symmetries and phase-diversity to achieve very fast WF reconstruction. However, FF approximates the pupil amplitudes as an even function that not necessarily matches exactly the real situation.

To improve the WF correction beyond the ac-

---

\* v.a.korkiakoski@tudelft.nl

curacy of FF, a natural way is to use approaches similar to the GS algorithm. However, the standard modifications of the algorithm are sensitive to the used phase diversities, in particular when the pupil amplitudes are not known, and they do not work with iterative wavefront correction as in FF. Therefore, our second algorithm combines FF and GS in a way that can be used not only to correct the wavefront, but also to estimate the pupil amplitudes – for which we make no assumptions. This comes at a cost in terms of noise sensitivity and instabilities as well as more demanding computational requirements.

At first, we illustrate the motivation and principles of the FF algorithm in Section 2. Then, Section 3 describes the Fast & Furious Gerchberg-Saxton (FF-GS) algorithm in detail. Section 4 describes the used hardware, Section 5 shows simulation and experimental results, and Section 6 draws the conclusions.

## 2. Fast & Furious

The Fast & Furious algorithm is based on iteratively applying a weak-phase approximation of the wavefront. The main principle of the weak-phase solution is presented in [16], but we found slight modifications [13] leading to significantly better performance. The algorithm uses focal-plane images and phase-diversity information to solve the wavefront, and the estimated wavefront is corrected with a wavefront correcting device. The correction step produces phase-diversity information and a new image that are again used to compute the following phase update. The schematic illustration of the algorithm is shown in Fig. 1.

An important aspect of the algorithm is to maximize the use of the most recent PSF – denoted as Image 1 in Fig. 1. In the weak-phase regime, a single image is sufficient to estimate both the full odd wavefront component and the modulus of the even component of the focal-plane electric field. The phase-diversity is needed only for the sign determination since we assume the wavefront aberrations are small. This makes the FF substantially less prone to noise and stability issues as compared to approaches relying more on the phase diversity information – such as the FF-GS.

Section 2.A explains the details of the weak-phase solution, and Section 2.B discusses the practical aspects when implementing the algorithm.

### 2.A. Weak-phase solution

A monochromatic PSF can be described by Fraunhofer diffraction and is given by the squared modu-

lus of the Fourier transform of the complex electric field in the pupil plane,

$$p = |\mathcal{F}\{A \exp(i\phi)\}|^2, \quad (1)$$

where  $A$  is the pupil amplitude describing transmission and  $\phi$  is the wavefront in the pupil plane.

The second order approximation of the PSF, in terms of the wavefront expansion, can be written as

$$p = |\mathcal{F}\{A + iA\phi - 0.5A\phi^2\}|^2. \quad (2)$$

The phase  $\phi$  can be represented as a sum of even and odd functions,

$$\phi = \phi_e + \phi_o, \quad (3)$$

and Eq. (2) can then be written as

$$p = |\mathcal{F}\{A + iA\phi_e + iA\phi_o - 0.5A\phi_e^2 - 0.5A\phi_o^2 - A\phi_e\phi_o\}|^2. \quad (4)$$

We make the assumption that  $A$  is even, and therefore all the terms here are either even or odd. Therefore, the corresponding Fourier transforms are then either purely real or imaginary with the same symmetries; we list the corresponding terms in Table 1.

Table 1. Notations and symmetries

| Aperture plane  |       |          | Fourier plane |           |          |
|-----------------|-------|----------|---------------|-----------|----------|
| Term            | Re/Im | Symmetry | Term          | Re/Im     | Symmetry |
| $A$             | real  | even     | $a$           | real      | even     |
| $A\phi_e$       | real  | even     | $v$           | real      | even     |
| $A\phi_o$       | real  | odd      | $iy$          | imaginary | odd      |
| $A\phi_e^2$     | real  | even     | $v_2$         | real      | even     |
| $A\phi_o^2$     | real  | even     | $y_2$         | real      | even     |
| $A\phi_e\phi_o$ | real  | odd      | $iz$          | imaginary | odd      |

Thus, all the introduced variables in Table 1 are purely real. The quantities  $a$ ,  $v$  and  $y$  denote the Fourier transforms of the pupil function, even and odd wavefront aberrations, respectively,

$$a = \mathcal{F}\{A\} \quad (5)$$

$$v = \mathcal{F}\{A\phi_e\} \quad (6)$$

$$y = \text{Im}\{\mathcal{F}\{A\phi_o\}\}. \quad (7)$$

Using the definitions, the second-order PSF approximation can be written as

$$p = |a + iv - y - 0.5v_2 - 0.5y_2 - iz|^2, \quad (8)$$

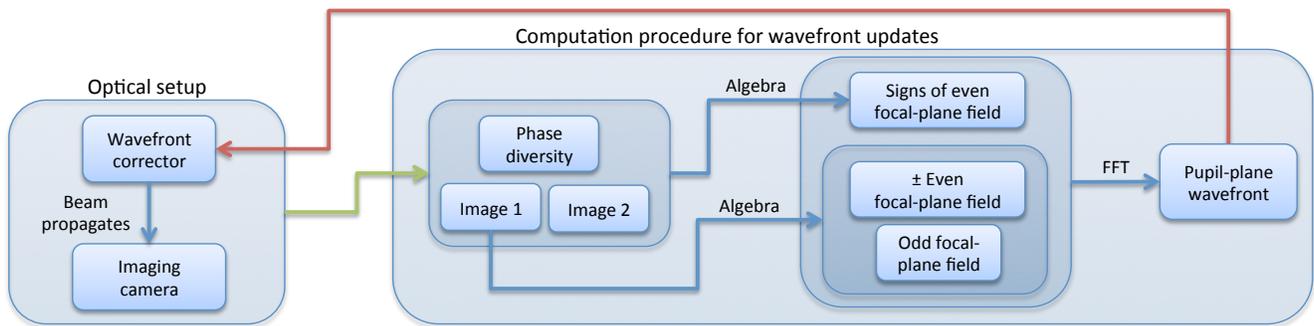


Fig. 1. Schematic illustration of the FF algorithm.

which simplifies to

$$p = a^2 + v^2 + y^2 - 2ay + \xi, \quad (9)$$

where the first four terms constitute the first order approximation – in terms of the wavefront expansion – and the second-order component is

$$\xi = 0.25v_2^2 + 0.25y_2^2 + z^2 - av_2 - ay_2 + 0.5v_2y_2 + yv_2 + yy_2 - 2vz. \quad (10)$$

The above equations are best illustrated by an example. We consider a purely sinusoidal wavefront having a peak-to-valley value of 1.0 rad and an rms error of 0.37 rad – alternative examples can be seen for instance in [17]. The wavefront and the resulting PSF image are shown in Fig. 2. The WF causes two main side lobes and more side lobes with significantly lower intensity; one pair is shown in Fig. 2.

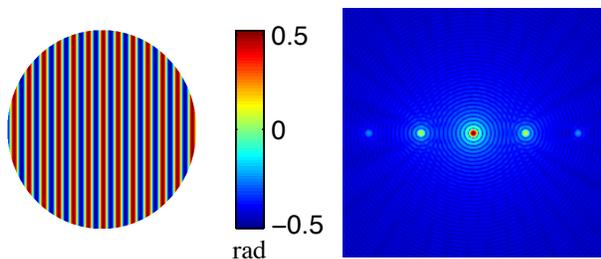


Fig. 2. Left: a purely sinusoidal wavefront. Right: resulting image raised to the power of 0.2 to compress the dynamic range.

Fig. 3 shows a radial cut of the second order component  $\xi$  for the example wavefront. Its most significant terms are  $av_2$  and  $ay_2$ , and therefore the perfect image ( $a^2$ ) scaled by a negative coefficient approximates  $\xi$  reasonably well. This term is responsible of the energy conservation by reducing the Strehl ratio [13]. The first-order approximation always has a Strehl ratio of 1.

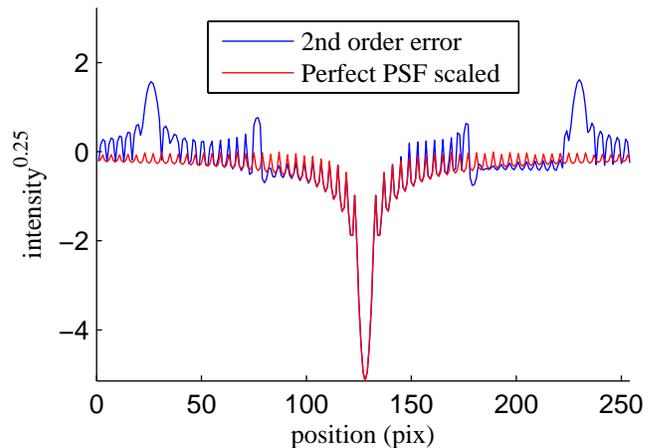


Fig. 3. Radial cuts of the second order component  $\xi$ , defined in Eq. (10), and an inverted and scaled perfect PSF,  $a^2$ .

Thus, an improved first order approximation can be obtained by subtracting a scaled version of  $a^2$  from the first order PSF approximation; the scaling coefficient needs to be adjusted such that the maxima of the perfect PSF and the approximation are the same. The radial cuts of the PSF approximations are illustrated in Fig. 4. The improved first-order approximation captures the main lobe and the first pair of side lobes quite well, but the secondary side lobes are missed.

However, for a wavefront with an rms error of less than one radian, the improved first-order approximation is often sufficient, and it can be formulated as

$$p = a^2 + y^2 + v^2 - 2ay - \left(1 - \frac{\max(p_n)}{\max(a^2)}\right) a^2, \quad (11)$$

where  $p_n$  denotes the recorded image normalized to

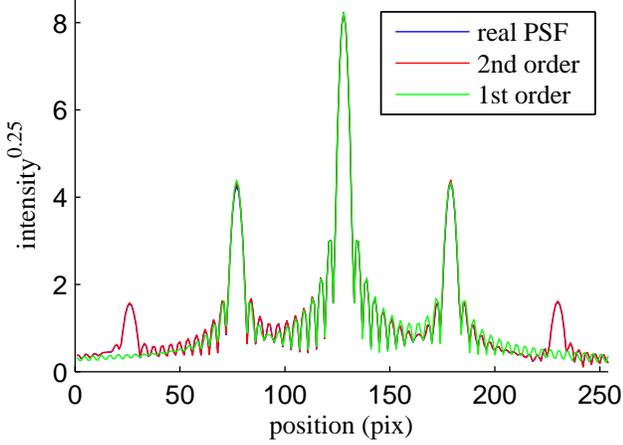


Fig. 4. Radial cuts of the perfect PSF, its improved 1st order approximation and the 2nd order approximation. The latter is virtually identical to the perfect PSF.

the same energy as the perfect PSF,

$$p_n = p_m \frac{\sum_{x,y} a^2(x,y)}{\sum_{x,y} p_m(x,y)}, \quad (12)$$

where  $(x, y)$  denotes the detector pixel coordinates and  $p_m$  is the raw image. Therefore, to simplify the notations, it is convenient to define a modified normalization of a PSF,

$$p' = p_n + \left(1 - \frac{\max(p_n)}{\max(a^2)}\right) a^2, \quad (13)$$

where the normalized image,  $p'$ , has the same maximum as  $a^2$ .

To solve the wavefront using Eq. (11), we follow the procedure of [16], which is repeated here for convenience.

The recorded image is normalized and broken to its even and odd parts. It then holds that

$$p'_e = a^2 + v^2 + y^2 \quad (14)$$

$$p'_o = 2ay. \quad (15)$$

The odd component of the wavefront is then easily reconstructed by first solving  $y$  using Eq. (15), and then using the inverse of Eq. (7). Due to noise and approximation errors, the direct application of Eq. (15), however, would result in division by excessively small values. We compensate this by using a regularization as in [16],

$$y = \frac{ap'_o}{2a^2 + \epsilon}, \quad (16)$$

where  $\epsilon$  is a small number. We found it best to set  $\epsilon$  to a value of 50–500 times the measured noise level of the recorded images.

To compute the even wavefront component, we need additional information in the form of phase diversity. We assume that a second, previously recorded image is known, and it was obtained with a known phase change compared to  $p$ . The even component of its normalized version can be written as

$$p'_{e2} = a^2 + (v + v_d)^2 + (y + y_d)^2, \quad (17)$$

where  $v_d$  and  $y_d$  are the even and odd Fourier components of the phase diversity, obtained in analogy to Eqs. (6) and (7).

Using Eqs. (14) and (17), we can solve  $v$  (the even phase component in Fourier space) and write it as

$$v_s = \frac{p'_e - p'_{e2} - v_d^2 - y_d^2 - 2yy_d}{2v_d}. \quad (18)$$

However, this formula is highly sensitive to noise due to the subtraction of two very similar images. Therefore, as also in [16], we use Eq. (18) only to compute the signs of  $v$ ; a more robust form follows from the use of Eq. (14),

$$v = \text{sign}(v_s) |p'_e - a^2 - y^2|^{0.5}, \quad (19)$$

where we use the absolute value to avoid taking the square root of negative values, occurring due to noise and approximation errors; this was observed to work better than zeroing the negative values. The even wavefront component is then computed in the same way as the odd one, by using Eq. (19) and the inverse of Eq. (6).

## 2.B. Practical aspects

To use the FF algorithm as presented here, it is necessary to have a wavefront correcting device – a deformable mirror or spatial light modulator – whose phase response is known. It is then possible to translate the desired phase change to appropriate wavefront corrector command signals. An appropriate mapping can be created using the standard adaptive optics calibration procedures as in [14] or, as we do here, with the help of dOTF based calibration method [15]. The method is based on determining the SLM phase (and transmission) response, when the control signal is changed in different pixel blocks. This data is then used to find an affine transform that maps the location of each SLM pixel to its physical location in the pupil plane.

We also assume that the collected images are sufficiently sampled: without aberrations the full

width at half maximum of the PSF has to be at least two pixels. If the detector is undersampled, aliasing prevents using the intensity images as described in Section 2.A. Large oversampling is also not desired since it increases the computational requirements.

The phase array,  $\phi$ , needs to be sampled with sufficient resolution to also model the pupil aperture,  $A$ , with good accuracy. The values we use ( $170 \times 170$ ) are sufficient for our purpose; we expect no significant sampling errors when implementing Eqs. (6) and (7) as fast Fourier transforms (FFTs). However, we need to zero-pad the recorded images such that the FFTs correctly implement the Fourier transforms in Eqs. (5), (6) and (7); the sampling of the arrays  $a$ ,  $v$  and  $y$  need to match the pixels of the camera. The amount of zero-padding is determined by the sampling coefficient,

$$q = \frac{N_{\text{arr}}}{N_{\text{pup}}}, \quad (20)$$

where  $N_{\text{arr}}$  is the dimension of the FFT array and  $N_{\text{pup}}$  is the size of  $\phi$ . We use the dOTF method as discussed in [15] to find  $q$ . The method is based on the use of localized phase diversity at the pupil border, which makes it possible to very straightforwardly create an array where the pupil shape can be directly seen. The parameter  $q$  is calculated by comparing the sizes of the pupil and the dOTF array.

When performing the FFT to obtain the phase from  $v$  and  $y$ , we combine the two real-valued FFTs to a single complex FFT [13],

$$A\phi = \mathcal{F}^{-1} \{w(v + iy)\}, \quad (21)$$

where  $w$  is a windowing function; it implements filtering necessary for numerical regularization – typically, high spatial frequencies are detected with higher uncertainty, and they need to be damped to obtain feasible reconstructions. The regularization is needed also with noiseless images since the weak-phase solution provides only approximate wavefronts. In this work, we have used a concave parabola, whose width can be adjusted depending on the noise level. An optimum filter is the subject of future studies.

To implement the iterative feed-back loop to optimize the wavefront error, we use a standard, leaky-integrator control. The wavefront-corrector shape at time step  $k$  is calculated as

$$\theta_k = g_l \theta_{k-1} - g A \phi_{k-1}, \quad (22)$$

where  $g_l$  is the leaky gain,  $\theta_{k-1}$  is the previous wavefront corrector shape,  $g$  is the integrator gain, and

$A\phi_{k-1}$  is the most recent small phase solution, computed using two most recent images using Eq. (21).

The integrator gain,  $g$ , determines the tradeoff between convergence speed and stability; a small gain results in slow convergence, a high gain means the image noise causes larger errors after the algorithm has converged. Excessively small gain would also make the use of phase-diversity information difficult.

The leaky gain is another regularization parameter. A value of  $g_l = 1$  would be equal to a standard integrator, and it would be optimal in the case of no errors, the equation  $p = |\mathcal{F} \{A \exp(i\phi)\}|^2$  perfectly describing the system. Values  $g_l < 1$  introduce wavefront aberrations at every time step preventing the system reaching a perfect state. However, that also prevents creeping instabilities from destroying the performance. The result is a stable convergence to a level with a slightly higher residual wavefront error.

### 3. Fast & Furious Gerchberg-Saxton

The obvious limitation of the FF algorithm is the assumption of the pupil amplitudes being even. This holds reasonably well for most of the optical systems having a circular shape, possibly with a central obstruction. However, to achieve the optimal focal-plane wavefront sensing with a high-order system not suffering from other limiting factors, it is necessary to consider imaging models where the pupil amplitudes can have an arbitrary shape.

We have approached the problem by combining the FF-style weak-phase solution and a version of the Gerchberg-Saxton (GS) algorithm. The new algorithm is referred to as FF-GS in the following.

As with the GS algorithm, we maintain an iteratively updated estimate of the unknown quantities – in our case the pupil amplitudes. The pupil amplitude estimate, phase diversities and the recorded images are used to calculate the focal-plane field; it requires three Fourier transforms and the use of the weak-phase approximation. Then, a Fourier transform is used to propagate the field to the pupil plane. The propagation results in improved estimates for the pupil-plane amplitudes and the wavefront. The schematic illustration of the FF-GS algorithm is shown in Fig. 5.

The FF-GS computation procedure forms a loop that could be iterated several times to obtain improved wavefront estimates. However, we found that in practice it is sufficient to run only two iterations before applying the wavefront correction with the obtained estimate. As with FF, the wavefront correction yields another image and phase-diversity

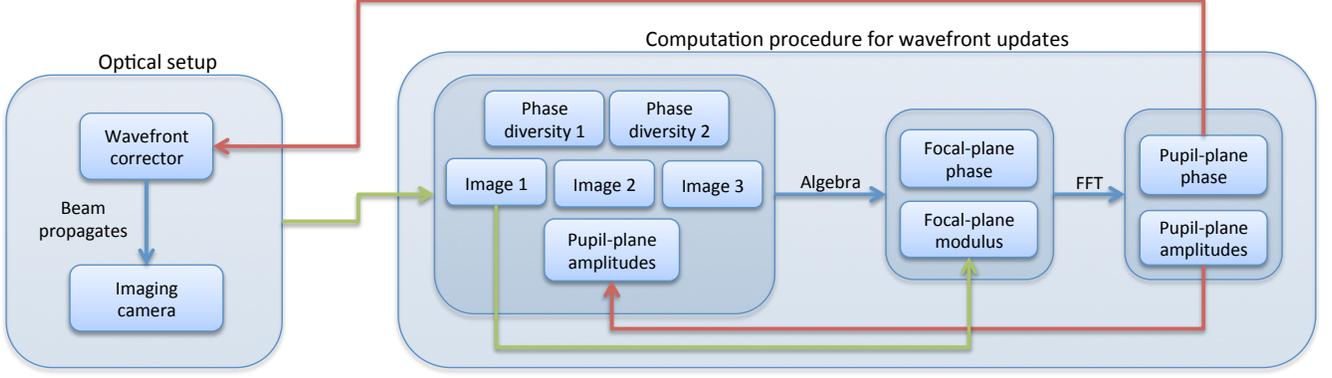


Fig. 5. Schematic illustration of the FF-GS algorithm.

information, which are used to compute the following correction step.

Next, Section 3.A describes the algebra that we use to compute the focal-plane electric field during the FF-GS procedure. Then, Section 3.B explains the details of the iterative computation, and Section 3.C discusses practical issues we face when implementing the algorithm.

### 3.A. A more general weak-phase solution

In this section, we assume that an approximation of the pupil amplitudes (denoted here as  $A$ ) is known; as a first step, a top-hat function is sufficient in the case of an unobstructed, round pupil. The estimates are updated iteratively, and we will make no restrictive assumptions about  $A$ .

We assume that three images are collected and that the corresponding phase-diversity information is known. The images are normalized according to Eq. (13), and it holds approximately that

$$p'_1 = |e_1|^2 = |\mathcal{F}\{A + iA(\phi)\}|^2 \quad (23)$$

$$p'_2 = |e_2|^2 = |\mathcal{F}\{A + iA(\phi + \phi_{d1})\}|^2 \quad (24)$$

$$p'_3 = |e_3|^2 = |\mathcal{F}\{A + iA(\phi + \phi_{d2})\}|^2, \quad (25)$$

where  $e_1$ ,  $e_2$  and  $e_3$  are the electric fields corresponding to the images,  $\phi$  is the unknown pupil-plane phase, and  $\phi_{d1}$  and  $\phi_{d2}$  are the known phase diversities applied to successively recorded images.

When counting the number of unknown variables, one can see that it might be possible to solve the unknown phase using only two images, with Eqs. (23) and (24). However, we found the following procedure with three images to be better. In addition of making the algebra easier, it is also significantly more robust since more information is available to compensate the errors in the estimate of  $A$ . Using even more images could potentially still improve the

results, but studying this is outside the scope of this paper.

Instead of solving the phase directly, we use phase-diversity information to find the electric field at the focal-plane. The electric field corresponding to Eq. (23) can be written as

$$e_1 = (a_r + \alpha) + i(a_i + \beta), \quad (26)$$

where

$$\begin{aligned} a_r &= \text{Re}\{\mathcal{F}\{A\}\} \\ a_i &= \text{Im}\{\mathcal{F}\{A\}\} \\ \alpha &= -\text{Im}\{\mathcal{F}\{A\phi\}\} \\ \beta &= \text{Re}\{\mathcal{F}\{A\phi\}\}. \end{aligned}$$

The unknown coefficients  $\alpha$  and  $\beta$  can be found by solving the equations that follow when subtracting Eq. (23) from Eqs. (24) and (25). The subtraction cancels all the non-linear terms and results in linear equations,

$$\begin{bmatrix} 2\alpha_{d1} & 2\beta_{d1} \\ 2\alpha_{d2} & 2\beta_{d2} \end{bmatrix} \begin{bmatrix} \alpha \\ \beta \end{bmatrix} = \begin{bmatrix} c_1 \\ c_2 \end{bmatrix}, \quad (27)$$

where

$$\begin{aligned} \alpha_{d1} &= -\text{Im}\{\mathcal{F}\{A\phi_{d1}\}\} \\ \beta_{d1} &= \text{Re}\{\mathcal{F}\{A\phi_{d1}\}\} \\ \alpha_{d2} &= -\text{Im}\{\mathcal{F}\{A\phi_{d2}\}\} \\ \beta_{d2} &= \text{Re}\{\mathcal{F}\{A\phi_{d2}\}\}, \end{aligned}$$

and

$$\begin{aligned} c_1 &= p'_2 - p'_1 - (2a_r\alpha_{d1} + 2a_i\beta_{d1} + \alpha_{d1}^2 + \beta_{d1}^2) \\ c_2 &= p'_3 - p'_1 - (2a_r\alpha_{d2} + 2a_i\beta_{d2} + \alpha_{d2}^2 + \beta_{d2}^2). \end{aligned} \quad (28)$$

We solve the coefficients  $\alpha$  and  $\beta$  by inverting the  $2 \times 2$  matrix in Eq. (27). The matrix has full rank, if the used phase-diversities are linearly independent. We found this generally to be the case when applying the algorithm, and therefore it was unnecessary to use any regularization methods. The coefficients can then be substituted into Eq. (26) to compute the focal plane electric field. However, this estimate would again be very prone to noise due to the subtraction of similar images, as shown in Eq. (28). Therefore, it is better to use the directly measured modulus and use only the phase-information following from Eq. (26). This then gives a more robust focal-plane estimate,

$$e_1 = |p'_1|^{0.5} \exp [i \arg((a_r + \alpha) + i(a_i + \beta))]. \quad (29)$$

The following section explains the details how this is then combined with the GS approach.

### 3.B. Iterative computation procedure

As the previous section indicates, we first record three images. The phase-diversity can be chosen freely, as long as its peak-to-valley stays below one radian. We use the FF algorithm at the initial steps.

Then, using the collected data, we perform computations to calculate a new wavefront update. The wavefront update is applied, and another image with different phase-diversity information is collected. The three most recent images are then used again to calculate the next phase correction to be applied. We continue until the algorithm converges.

The computation consists of a cycle of two successive GS-like iterations. The complete process consists of the following steps:

1. Take the pupil amplitudes,  $A$ , estimated at the previous iteration. Use the procedure in Section 3.A to calculate the focal-plane electric field corresponding to  $p_2$ , the second most recent image. This is done by solving  $\alpha$  and  $\beta$  in Eq. (27) and using formula

$$e_2 = |p'_2|^{0.5} \exp [i \arg((a_r + \alpha) + i(a_i + \beta))].$$

Here, the images could be rearranged appropriately:  $p_2$  should be the reference and the phase diversities interpreted accordingly. However, we found  $\arg(e_2) \approx \arg(e_1)$  to be a sufficient approximation.

2. Compute the pupil-plane electric field corresponding to the image  $p_2$ . This is done by Fourier transforming the focal-plane field,

$$E_2 = \mathcal{F}^{-1} \{e_2\}.$$

3. Update the current estimate of the pupil amplitudes:

$$A = |E_2|.$$

4. With the new pupil amplitude estimate, repeat the procedure in Section 3.A to compute the electric field for image  $p_1$ , the most recent image.

5. Compute the pupil-plane field corresponding to image  $p_1$ ,

$$E_1 = \mathcal{F}^{-1} \{e_1\}.$$

6. Calculate the final phase estimates for the phase and pupil amplitudes,

$$\phi = \arg(E_1) \quad (30)$$

$$A = |E_1|. \quad (31)$$

The estimates of  $\phi$  are then used in the feedback loop in the same way as with the FF algorithm.

### 3.C. Practical aspects

The issues faced in practice by an implementation of the FF-GS differ slightly from the simple FF.

Since the pupil amplitudes are not constrained, the imaging model is potentially much more accurate. In practice, indeed, we found that it was not necessary to apply any windowing filters to dampen the high spatial frequencies in the wavefronts reconstructed with FF-GS. The normal feed-back loop, as described by Eq. (22), was sufficient regularization for the optimal performance.

It was also not necessary to introduce any ad-hoc restrictions to constrain the pupil amplitudes. The values obtained from Eq. (31), at any time step, do have a significant deviation from the actual pupil amplitudes, but this appears to be a minor issue for the convergence of the algorithm. Moreover, averaging the values of  $A$  over several iterations produces non-biased results.

However, the heavier reliance on the phase-diversity information makes the algorithm more prone to stability issues. To increase the stability, we found it helpful to introduce other ad-hoc techniques.

In the feedback loop, we apply amplitude gains. Just as formulated in Eq. (22), we multiply the applied phase correction – obtained from Eq. (30) – by the estimated amplitudes. This helps to prevent abrupt phase changes at points where  $|E_1|$  has a very small value; at those points, the determination of the complex phase is likely to fail. In fact,

we also set  $\phi$  to zero at points where  $|E_1| < 0.3$ . This reduces the speed of convergence, but has no impact on the accuracy of the converged solution.

Finally, additional regularization is used in case of numerical issues when the algorithm has converged. We observed that occasionally, every 10th iteration or so, the FF-GS algorithm produces wildly incorrect results. This is related to the fact that the solution of Eq. (27) requires phase-diversity information. Once the applied phase corrections become very small, the corresponding diversity information becomes unreliable.

To make sure that such violent phase changes will not cause troubles, we simply restrict the magnitude of the applied phase change. If the rms value of the change exceeds the mean of ten previous changes, we scale it down to the mean value.

#### 4. Hardware used

To test the algorithms, we created a simple setup that consists of one spatial light modulator (SLM) and an imaging camera. The former is a reflective device (BNS P512) having a screen of  $512 \times 512$  pixels, a fill factor of 83.4% and a pixel pitch of  $15 \times 15 \mu\text{m}$ . The SLM is able to create a phase-change of  $2\pi$  radians at the used wavelength, and its control signal is coded with 6 bits.

The imaging camera is a Basler piA640-210gm, which has a resolution of  $648 \times 488$  pixels and a dynamic range of 12 bits. As a light source, we use a fibre-coupled laser diode (Qphotonics QFLD-660-2S) having a wavelength of 656 nm.

A schematic figure of the setup is shown in Fig. 6. The beam goes first through a diaphragm, and it is then collimated such that it hits an area of  $245 \times 245$  pixels on the SLM. The device reflects several sub-beams due to strong diffraction effects, and we use only the zeroth order beam; it is directly imaged onto the camera (beam numerical aperture  $\text{NA}=0.037$ ). The other sub-beams cause no adverse effects. Before and after the SLM, we place two linear polarizers that are rotated such that their orientation matches the one of the SLM.

The SLM phase and transmittance responses are measured with the differential optical transfer function (dOTF) method as described in [15]. The resulting measurements are shown in Fig. 7. The maximum control voltage causes  $\sim 2\pi$  phase shift at 656 nm.

The used SLM couples the transmittance and phase change; the transmittance gradually increases when a larger phase shift is introduced with the SLM. For phase changes of less than one radian, the transmittance is  $\sim 25\%$  lower compared

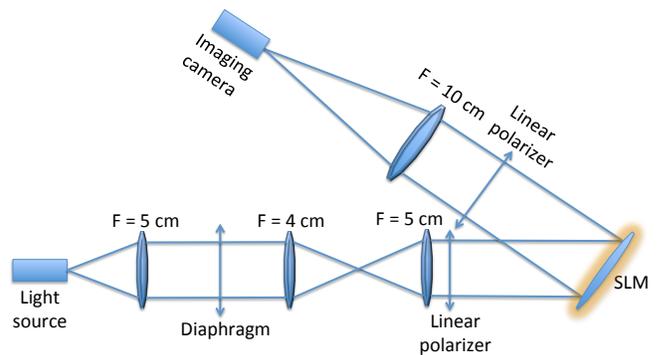


Fig. 6. Schematic view of the used hardware. The lenses are standard 1-inch doublets. The beam diameter is 3.7 mm at the SLM.

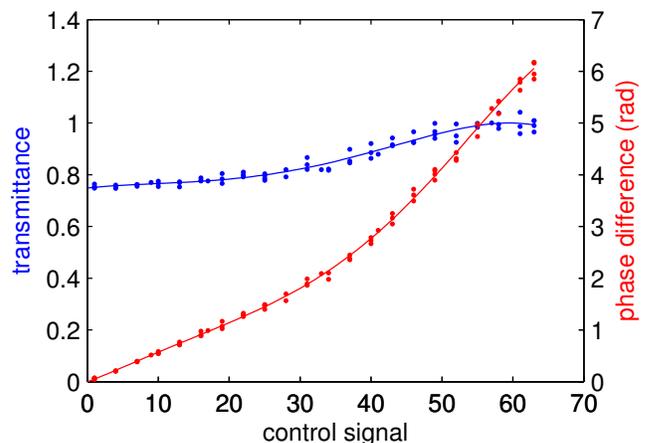


Fig. 7. SLM phase and amplitude responses. The dots indicate individual measurements. The lines show 5th order polynomial fits to the data.

to what is seen when a change of more than  $\sim 4$  rad is introduced.

To create a mapping between the pupil-plane coordinates and the SLM pixels, we again use the dOTF method and affine transforms as described in [15]. This time, however, we make the dOTF recording in the best focus to avoid issues with the non-telecentric beam. To compensate for signal-to-noise problems, we take more images to average out the noise: it takes  $\sim 2$  hours to create one dOTF array. This makes the process also more vulnerable to internal turbulence in the setup; the recorded images are blurred such that the low spatial frequencies in the images become distorted, and we have to mask out the center of the obtained dOTF arrays.

Fig. 8 shows the modulus of the best-focus dOTF array recorded with the whole SLM at zero control

voltage. Although the center of the array is masked, it is still perfectly usable for the calibration process of [15], and we can accurately determine the PSF sampling as defined by Eq. (20):  $q = 3.76 \pm 0.01$ .

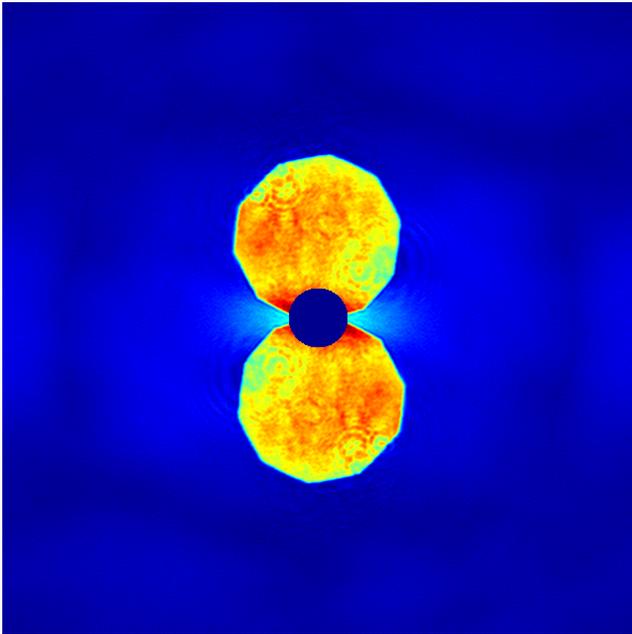


Fig. 8. The modulus of an averaged dOTF array.

The resulting SLM calibration is valid as long as the position of the SLM stays fixed with respect to the imaging camera, and the phase-response of the device does not change. In our setup, we found this to be case for at least one month – from the initial calibration to the last measurements reported in this paper.

As discussed in [15], the resolution of the controlled phase is a free parameter when calculating the affine mapping for the SLM calibration. We obtained good results when using  $\sim 30\%$  less pixels than are actually used by the SLM. Thus, we selected the size of the controlled phase array as  $N_{\text{pup}} = 170$ . The resulting FFT array dimension is then  $N_{\text{arr}} = 640$ .

When recording images for the FF and FF-GS algorithms, we use the same high-dynamic range (HDR) imaging approach as in [15]. Several snapshot images are taken with different exposure times, and we combine the images to extend the dynamic range and compensate noise. Each single-exposure component in one HDR image is an average over 40–200 images, and we used in total 16 exposure times (2, 5, 12, 25, 50, 100, 200, 400, 750, 1100, 1450, 1800, 2150, 2500, 2850 and 3200 ms). It took  $\sim 15$  s to record one HDR image. Increasing the

integration even further does not significantly improve the performance of the wavefront correction algorithms.

Although the imaging camera has a resolution of  $640 \times 480$  pixels, we use only a smaller area for convenience reasons. After acquiring the image, we crop an array of  $320 \times 320$  pixels such that the PSF maximum is in the center. Outside of the region, we did not observe any significant amount of light.

To detect all the spatial frequencies corrected by the controlled phase array of  $170 \times 170$  pixels, however, we would need an array of  $640 \times 640$  pixels. Thus, it is possible that our control algorithms introduce high-spatial frequencies that scatter light outside of the observed image. However, with FF, this is mitigated by the applied low-pass filter. With FF-GS, we observed no stability issues with the high spatial frequencies, although no explicit regularization measures were taken.

## 5. Results

This section illustrates the results of the FF and FF-GS algorithms. We consider only a single case: the wavefront to be corrected is what the camera sees at the beginning, when no voltage is applied to the SLM. We call this the initial situation.

We concentrate on the ultimate accuracy the algorithms can achieve in a low-noise regime. Our earlier publication [14] describes in more detail the FF performance in the presence of more noise. We showed that the algorithm works, but only the lower spatial frequencies can be reconstructed. Now, we study a case that is typical for a high-order adaptive optics test bench, and the noise level is chosen such that FF-GS offers an advantage over FF – with higher noise FF is more robust.

Section 5.A illustrates the properties of the converged algorithms as measured with our test setup. Section 5.B shows a more detailed comparison of the measurements and simulations with the actual hardware modeled in sufficient detail. Finally, Section 5.C presents a simulation-based error budget that quantifies the effects of different error sources.

### 5.A. Performance of the algorithms

For the results shown here, we have optimized the free parameters (FF regularization coefficient  $\epsilon$ , the width of the FF filtering window  $w$ , leaky gain  $g_l$ , loop gain  $g$ ) such that the converged WF quality is best; the convergence speed has lower priority.

The width of the filtering window used by the FF algorithm was chosen to be  $320 \times 320$ , the same as the recorded images. However, during the first 10 iterations, we used a narrower window (width of

80 pixels) to avoid introducing errors at the high spatial frequencies. After the lower spatial frequencies are corrected, it is safe to increase the window size.

The optimal values for feedback loop gains were  $g = 0.3$ ,  $g_l = 0.97$  (with FF) or  $g_l = 0.999$  (with FF-GS), and  $\epsilon$  was 250 times the determined noise level in the images.

For the FF algorithm, we also need to determine the pupil amplitudes,  $A$ . We use a perfect top-hat function having a size of  $N_{\text{pup}} \times N_{\text{pup}}$ , where the choice of  $N_{\text{pup}}$  is explained in Section 4. It might be possible to improve the results by adjusting  $A$  based on the actual pupil shape, but this is outside the scope of this paper.

With these settings, both FF and FF-GS converge in 20–50 iterations to a situation where the Strehl ratio has increased from  $\sim 75\%$  to  $\sim 99\%$  (a more detailed analysis can be found in Section 5.B). After the convergence, the control law, Eq. (22), gives phase updates that are negligible compared to the shape of the wavefront corrector,  $\theta_k$ . However, we run the algorithm for a total 400 iterations to make sure that no creeping instabilities occur.

Fig. 9 illustrates the typical wavefronts we obtained after the convergence. Due to the applied low-pass filter, FF yields wavefronts smoother than FF-GS; otherwise they match well, though. The repeatability of the experiments appears reasonable: the converged wavefront shapes have experiment-to-experiment differences at most  $\sim 0.2$ – $0.3$  rad. The spread of the FF-GS results tends to be smaller compared to FF, and we see that also the higher spatial frequencies are produced in a repeatable way.

Fig. 10 shows the reconstructed pupil amplitudes. The top left shows an average of  $A$  following the application of Eq. (31) during a total of 400 FF-GS iterations with phase updates. It can be compared with the dOTF modulus shown next to it, and we see that the shape of the diaphragm and several bigger dust particles are correctly recovered. However, it is obvious that all the finer details are lost, and the very lowest spatial frequencies also deviate from each other. The plot below in Fig. 10 shows radial cuts of five similarly obtained pupil amplitudes, and we see that all the features in the pupil amplitudes are nevertheless repeatedly reconstructed in the same way.

To obtain an improved reconstruction of the finer details in the pupil amplitudes, we use the PSF that results after the FF-GS algorithm has converged. We assume that all the remaining speck-

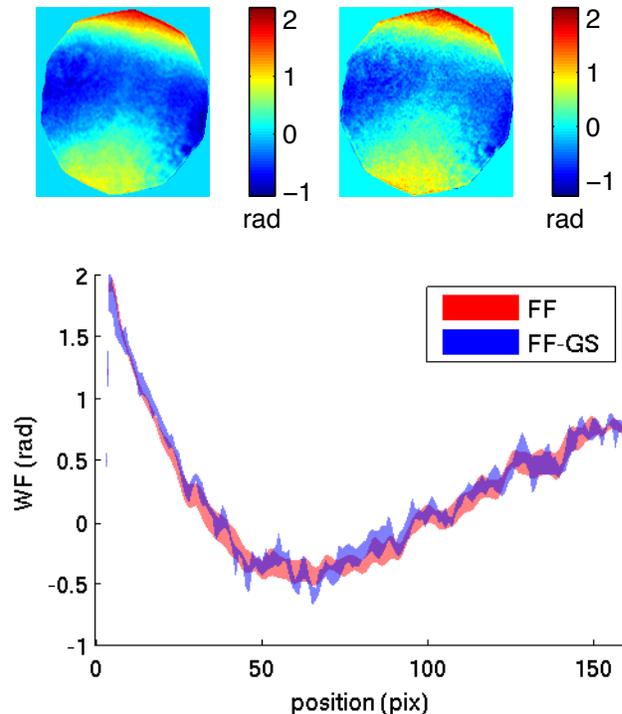


Fig. 9. Top row: typical wavefront shapes ( $170 \times 170$  pixels) of the SLM after the convergence of FF and FF-GS. Bottom: radial cuts through the wavefronts; the shaded area shows the range (minima and maxima) of five independent measurements.

les are caused by the amplitude aberrations, and reconstruct – with a Gerchberg-Saxton-style algorithm – a pupil that would create such a pattern. This is shown in the upper right in Fig. 10, and we can see that it indeed much better matches the dOTF reconstruction in Fig. 8. Later, we use this pattern in simulations for analysis purposes.

The differences between the independent measurement series shown here are a combination of actual small changes in the hardware and uncertainty caused by noise and systematic errors. It is difficult to separate those two effects, and therefore we continue the analysis with the help of numerical simulations.

### 5.B. Comparison of measurements and simulations

To simulate the optical setup, we assume that the algorithms correct wavefronts shown in Fig. 9 with pupil amplitudes similar to what is shown in Fig. 10. We created three study cases reflecting the variability in the converged results.

In the simulations, we consider eight different sources of errors that needs to be modeled explic-

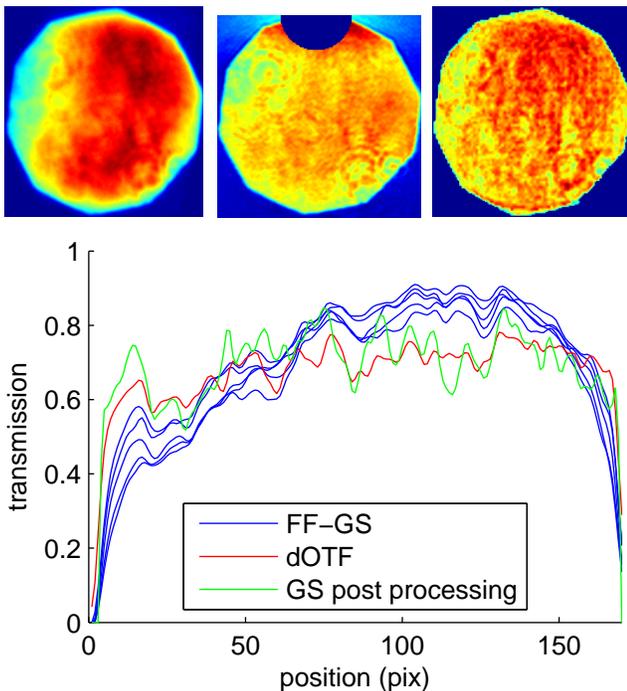


Fig. 10. Top row: pupil amplitudes ( $170 \times 170$  pixels) reconstructed with different methods. Left: FF-GS. Middle: dOTF (same as in Fig. 8). Right: GS post-processing from a converged PSF. Bottom: radial cuts through the pupil amplitudes; five independent measurements runs shown for FF-GS.

itly. They are:

1. SLM quantification. We use only 6 bits to control the wavefront. The plots shown in Fig. 7 are used to round the simulated WF correction to what would happen in practice.
2. PSF sampling. The wavefront and the resulting PSF are sampled internally by a factor of two higher than what the hardware controls or observes. The control algorithms use re-binned PSFs, and the simulated wavefront correction is interpolated bilinearly from the reconstruction at a resolution of  $170 \times 170$ .
3. Image noise and dynamic range. We estimate the read-out noise of the HDR images to be at a level of  $2.2 \cdot 10^{-6}$  of the image maximum. Gaussian random noise is added to the simulated PSFs. The HDR images have maximum values  $\sim 4 \cdot 10^8$ , corresponding to about 29 bits, and this is also modeled in the simulations.
4. Background level. Standard background subtraction is performed on the PSF images, but a small error will still remain. Therefore, we

add a constant background level,  $2.7 \cdot 10^{-6}$  of the image maximum, to the simulated PSFs.

5. Non-perfect pupil. Instead of the perfect top-hat function, we use pupil amplitudes similar to what is illustrated in the top right of Fig. 10.
6. Amplitude aberrations. We simulate the coupling of the wavefront and the transmission of the SLM as illustrated by Fig. 7.
7. Alignment errors. Although the dOTF calibration is rather accurate, some error could still be present in the affine transform that we use to map the wavefront to the SLM pixels. The simulations indicate that if the transform has a mismatch corresponding to a rotation larger than  $0.4^\circ$ , FF and FF-GS would be unstable. In practice, with the used hardware, we saw no hints these of instabilities. Therefore, a rotation error of  $0.4^\circ$  represents the maximum misregistration that the wavefront control algorithms are likely to experience.
8. Tip-tilt error. Internal turbulence in the optical setup causes frame-to-frame wavefront variations, which can be approximated to a degree as small shifts of the recorded images. We measured the difference of the center-of-gravity between two consecutive PSFs recorded with the HDR method, and it was found to be on average 0.025 pixels. This error cannot be taken into account by the phase-diversity approach, and we model its impact on the performance.

Fig. 11 shows the remaining wavefront error as a function of time step. The simulation plots show the exact error, but the measured value is estimated from the data. Here, we have estimated the rms error from the corresponding PSF images only. At first, we estimated the Strehl ratios using the method seven in [18], and the result was converted to an rms error using the expression  $S = \exp(-\sigma^2)$ . The resulting estimates are highly sensitive to the estimation of the pupil amplitudes, which we know only approximately (Fig. 10). Thus, the y-axis in the lower plot in Fig. 11 is not directly comparable to the simulation plot; alternative estimates that are more easily compared are shown later in this Section.

Nevertheless, the speed of the convergence is clearly seen. Both FF and FF-GS reduce the WF rms error from  $\sim 0.5$  rad rms to  $\sim 0.1$  in  $\sim 50$  iterations. FF converges about 50% faster, but it is

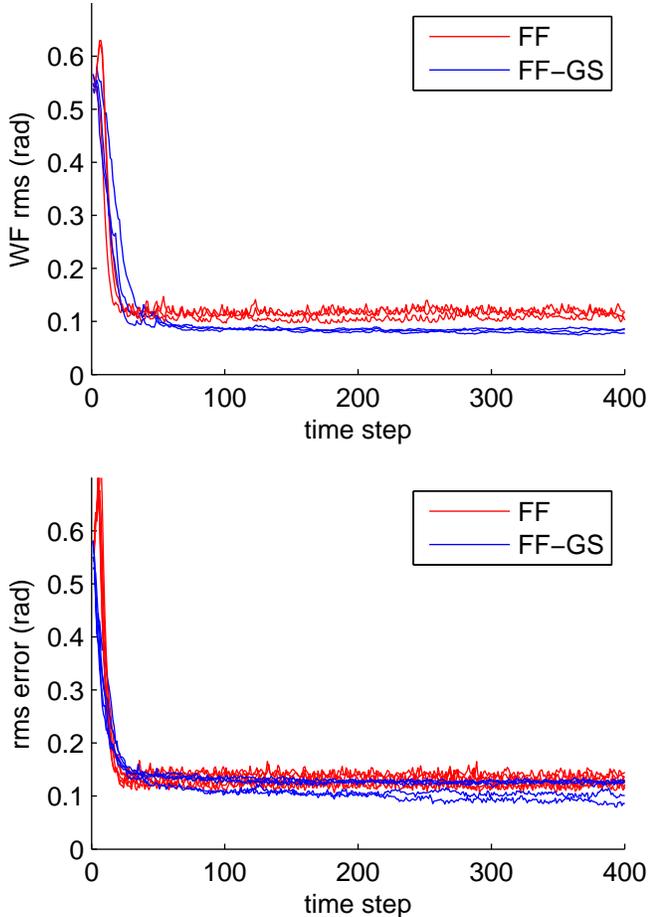


Fig. 11. Tip/tilt removed residual wavefront error as a function of time step. Top: simulations (real value). Bottom: measurements (estimation from PSF images).

plagued by the overshoot at the beginning; it would require an adaptive optimization of the low-pass filter to properly handle it.

Regarding the simulations, it is obvious that the FF-GS improves the performance over FF: the rms error is 0.08 rad as compared to 0.12 rad. This is largely due to the smaller value of the leaky integrator gain that we had to apply to make the FF stable.

Regarding the measurements, we can see a similar pattern, but we also see that the FF-GS has two modes: the estimate of the residual rms error is either  $\sim 0.10$  rad or  $\sim 0.13$  rad. The modes are related to the finite sampling of the CCD detector. Our models do not explicitly constrain the position of the PSF at the detector, which means that a random sub-pixel tip/tilt component – different between the independent measurement series – is left in the residual wavefront. The algorithms con-

verge to a state that remains stable, but the different remaining tip/tilt components can cause significant changes in the measured maximum intensity, and this affects our Strehl ratio estimation process. When inspecting the re-centered PSFs carefully, as shown later in this section, no significant differences between the PSFs can be seen.

A more detailed investigation reveals that the convergence of the wavefront correction depends on the spatial frequency – low-frequency features are reconstructed faster. Fig. 12 illustrates this by showing how an average intensity in different regions of the field changes as a function of time step. We show three different regions representing low, medium and high spatial frequencies; the locations correspond to Airy rings 2–4, 12–17 and rings further than 30. Since we consider only small wavefront aberrations, the shown intensity values are directly proportional to the average power spectral density at the matching frequency bands.

Both simulations and measurements show a similar pattern, although the absolute levels are higher in simulations due to differences in noise. At low spatial frequencies, both FF and FF-GS peak at iterations 5–10. FF converges in total in  $\sim 20$  iterations, and FF-GS takes  $\sim 20$  iterations more, although some cases show intensity reduction even until  $\sim 100$  iterations. At medium spatial frequencies, the peak occurs at iteration  $\sim 15$ , and the algorithms need in total  $\sim 30$  iterations to reach intensity level  $\sim 6\%$  lower than at the beginning. FF saturates at that level, but 30 additional iterations with FF-GS reduce the intensity in total  $\sim 15\%$  from the initial level. At high spatial frequencies, FF requires almost 50 iterations to converge to a level 15% lower than the initial intensity (in simulations the reduction is only a few percentages due to higher noise). FF-GS, on the other hand, converges faster than FF, but still 150 iterations are needed to reduce the intensity  $\sim 35\%$ . The measurements show marginally better intensity reduction, but that requires almost 300 iterations.

The residual wavefront error can obviously also be estimated using the control data that the algorithms themselves provide through Eqs.(21) and (30); the corresponding results are shown in Fig. 13.

The first striking feature is that the simulations and the measurements produce practically identical patterns. After the convergence, the WF estimates of the FF algorithm have an rms error of 0.12–0.18 rad in the simulations and 0.15–0.24 rad in the measurements. There appears to be no obvious structure in how the error varies between con-

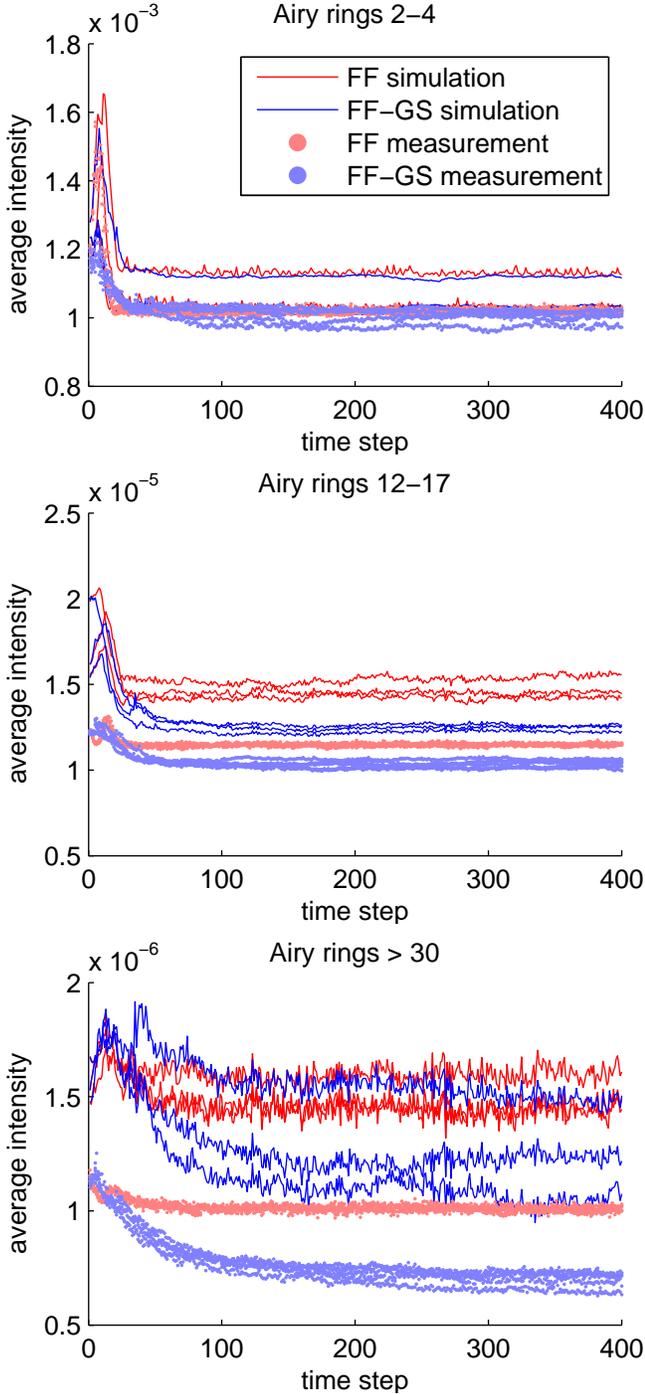


Fig. 12. Average intensity at different parts of the field. Three cases are shown: the field corresponding to Airy rings 2–4, Airy rings 12–17 and Airy further than 30.

secutive iterations. Since the actual correction is an average over several consecutive measurements, the actual remaining wavefront error can be smaller than the instantaneous estimates of 0.12–0.24 rad. In the simulations, the error was observed to be

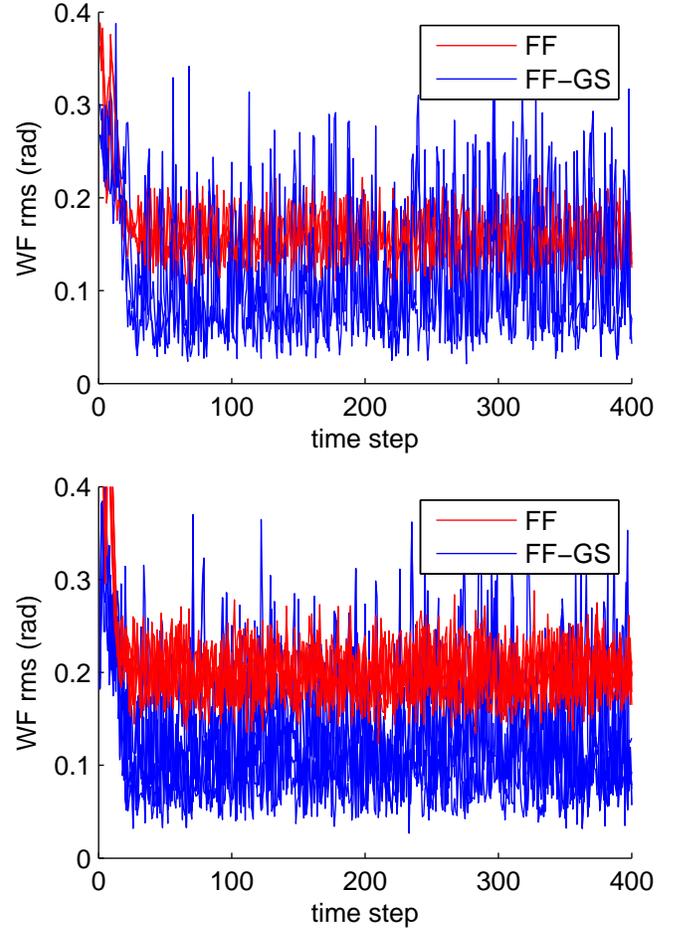


Fig. 13. Residual wavefront error as a function of time step. Values calculated from the actual estimates used by the algorithms. Top: simulations. Bottom: measurements.

$\sim 0.12$  rad, and we have no reason to assume the situation with the actual hardware would be different; our estimate for the remaining WF rms error is  $\sim 0.15$  rad.

With the FF-GS algorithm, the issue is slightly more complicated since some of the WF estimates fail when the algorithm approaches the optimum. The reason for this – the phase-diversity failure – is discussed in Section 3.C. This is seen as prominent spikes in the plots in Fig.13, although most of the rms error values are concentrated around 0.1 rad. In the simulations, the actual rms error of the residual wavefront is  $\sim 0.08$  rad, and a similar value is seen in the actual measurements.

Four examples of the actual PSF images are shown in Fig. 14:

1. the initial PSF (measured when the SLM pixels are set to zero),

2. the simulated perfect PSF resulting from the pupil amplitudes shown in Fig. 10,
3. simulated PSF after the convergence of the FF-GS algorithm,
4. measured PSF after the convergence of the FF-GS algorithm.

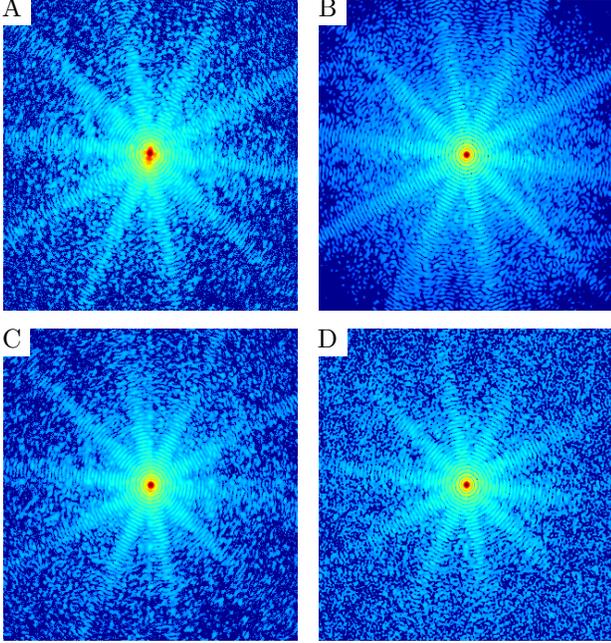


Fig. 14. Examples of PSF images ( $320 \times 320$  pixels) raised to the 0.1 power. A) initial, measured. B) perfect, simulated C) converged FF-GS, measured. D) converged FF-GS, simulated.

All the PSFs have a similar, star pattern with ten radial beams gradually fading towards the edges of the images. These are caused by the blades of the diaphragm, whose shape is shown in Figs. 8 and 10.

The initial PSF corresponds to a wavefront like in Fig. 9: a clearly deformed core, but still easily recognizable Airy rings 3–20.

The simulated, noiseless and aberration-free PSF shows the speckles that we expect to remain due to the non-flat pupil amplitudes. The dust, dirt and also the inhomogeneities of the SLM create a significant transmission distortion dominated by high spatial frequencies. This causes the halo of irregularities on top of the pattern of the perfect diffraction rings. In addition, we can see a few stronger speckles and speckle groups at a distance of approximately Airy rings 12–18. These can be attributed to the larger dust particles also clearly visible in the FF-GS estimated pupil amplitudes in Fig. 10.

When comparing the measured and simulated PSFs after the FF-GS algorithm has converged, we find no significant differences. Both PSFs have a regular core, which appears to match exactly the perfect PSF up to the 4th diffraction ring. At least 26 diffraction rings are, at least partially, visible. A comparison with the perfect PSF shows that several strong speckles can be identified in all the images, but the halo after the 14th diffraction ring outside the star-like beams, close to the detection limit of the camera, is dominated by speckles with no obvious structure.

A more detailed comparison can be obtained by inspecting the radially averaged profiles of the PSFs. Before taking the radial average, we shift, using Fourier transforms, the PSFs to have the center-of-gravity at the location of the perfect PSF. The results are shown in Fig. 15.

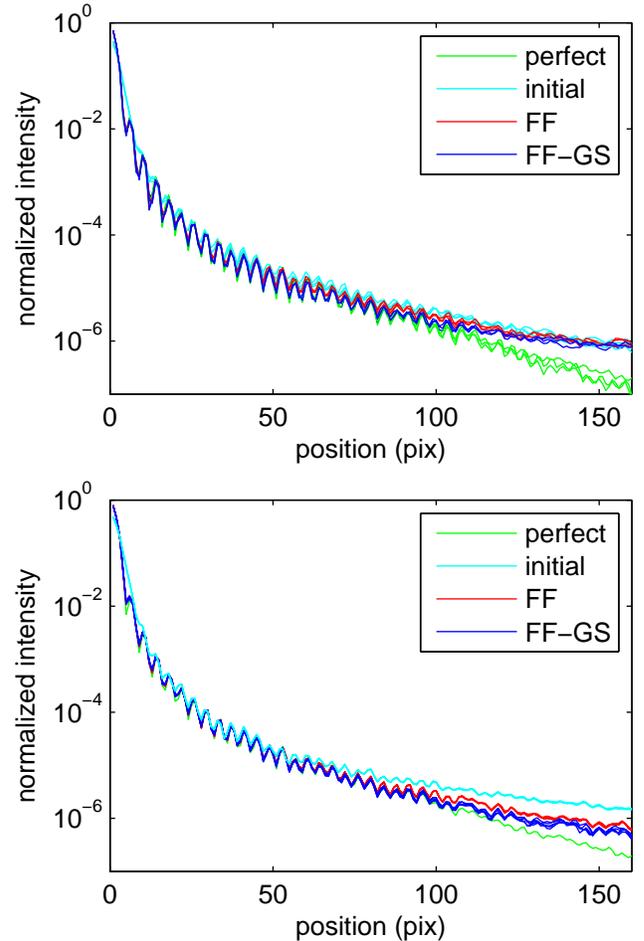


Fig. 15. Averaged radial profiles of PSF images. Upper: simulated, the three study cases are shown. Lower: measured, results from five independent runs are shown; the perfect PSF is identical to the one in the upper plot.

The profiles show that both the FF and FF-GS algorithms, in both the simulated and measured cases, converge to a situation very close to the perfect simulated PSF; no significant differences are seen up to the first 13 (simulated) or 20 (measured) diffraction rings. After this, we can see that the performance of both algorithms slowly deviates from the perfect PSF, the intensity being a factor of  $\sim 5$  (simulated) or  $\sim 2-3$  (measured) higher at borders. At the distances corresponding to diffraction rings 20 and higher, FF-GS is typically  $\sim 20-30\%$  better in reducing the intensity as compared to FF.

In total we can recognize at least 30 diffraction rings before the speckle noise makes the PSF structure too blurry to observe any structure. Nevertheless, compared to the initial PSF, both algorithms reduce the intensity of scattered light throughout the whole used field, although, in the simulated case, the difference is not significant after the 34th diffraction ring. In the measured case, on the other hand, the light intensity is reduced by a factor of  $\sim 2-3$  also at the edge of the recorded image. This difference between the simulations and measurements is due to a combined effect of differences in actual noise levels, wavefronts and pupil transmission.

### 5.C. Error budget

Finally, we show an error budget that illustrates the impact of the different error sources in the optical setup.

In the ideal case, we have no noise and a perfectly circular pupil that is – in the case of FF – exactly known. The perfect case also uses exactly the same imaging model in both the WF reconstruction and when simulating the PSF images: a zero-padded FFT with a wavefront modeled at a resolution of  $170 \times 170$ .

We sequentially simulate each of the error sources listed in Section 5.B. The resulting rms errors in the converged wavefronts are listed in Table 2.

In theory, both algorithms should reach zero wavefront error in the perfect case. However, in the case of FF, we still have to use numerical regularization to maintain stability, and this compromises the performance in the error-free case. This could be improved by optimizing the codes, but it is not done here; the codes are optimized for the performance with all the error sources present.

The most severe error source for the FF algorithm, as expected, is indeed the amplitude aberrations: instead of the ideal rms error of 0.03 rad, we are limited to an error of 0.11 rad. Similar errors

Table 2. Error budget

|                          | FF*             | FF-GS*          |
|--------------------------|-----------------|-----------------|
| 0. No errors             | $0.03 \pm 0.01$ | $0.00 \pm 0.00$ |
| 1. SLM quantification    | $0.04 \pm 0.01$ | $0.02 \pm 0.00$ |
| 2. PSF sampling 2x       | $0.08 \pm 0.01$ | $0.01 \pm 0.00$ |
| 3. Image noise           | $0.05 \pm 0.01$ | $0.05 \pm 0.00$ |
| 4. Background level      | $0.04 \pm 0.01$ | $0.01 \pm 0.00$ |
| 5. Non-perfect pupil     | $0.11 \pm 0.00$ | $0.02 \pm 0.01$ |
| 6. Amplitude aberrations | $0.12 \pm 0.01$ | $0.04 \pm 0.01$ |
| 7. Alignment errors      | $0.08 \pm 0.01$ | $0.01 \pm 0.00$ |
| 8. TT instability        | $0.03 \pm 0.01$ | $0.04 \pm 0.01$ |
| 9. All errors            | $0.12 \pm 0.01$ | $0.08 \pm 0.00$ |

\*The residual WF rms errors (rad) at spatial frequencies falling within the used images.

are also seen if the imaging model does not exactly match the actual hardware; this was tested when simulating the wavefront and PSF with double sampling (case 2 in Table 2); the double sampling was also used in the misalignment simulation. The different error sources are coupled, so they do not add up quadratically. In the presence of all the error sources, we end up having a residual WF error of  $\sim 0.12$  rad.

With the FF-GS algorithm, we can radically reduce the problems of the unknown pupil aberrations. The transmission we used in simulations, however, had significant fluctuations creating speckles similar to what the wavefront aberrations do. Therefore, the wavefront reconstruction problem is difficult to make unambiguous, and we saw a small residual rms error of 0.02 rad.

The FF-GS is limited by the combined effect of read-out noise (0.05 rad), the fact that the SLM couples the transmission and phase change (0.04 rad) and the TT instability (0.04 rad). All the error sources add up quadratically, which indicates that they are largely independent.

When comparing the FF and FF-GS, we see that a significant improvement can be obtained with the FF-GS algorithm; the residual wavefront rms error is reduced from 0.12 rad to 0.08 rad. However, the method is more sensitive to uncertainties and noise: the tip-tilt jitter in our hardware has no influence on the FF while being a major error source with the FF-GS algorithm.

## 6. Conclusions and discussion

We have demonstrated the performance of two numerically efficient focal-plane wavefront sensing algorithms: the Fast & Furious and its extension Fast

& Furious Gerchberg-Saxton.

Both algorithms do an excellent job in calibrating static aberrations in an adaptive or active optics system: we demonstrated an increase in the Strehl ratio from  $\sim 0.75$  to  $0.98$ – $0.99$  with our optical setup.

Although the FF-GS algorithm is more prone to noise, we observed a clear improvement. With our hardware – a high-resolution spatial light modulator as the wavefront corrector – we estimate the remaining residual wavefront rms error to be  $\sim 0.15$  rad with FF and  $\sim 0.10$  rad with FF-GS. The difference occurs mostly at spatial frequencies corresponding to the 20th and further Airy rings.

Simulations with error sources comparable to our hardware show very similar results. This increases our confidence that the estimated performance indicators are reliable, and the simulated error budget also confirms the unknown amplitude aberrations as the main limitation of the FF algorithm in the considered framework.

To our knowledge, this is the first time that such focal-plane sensing methods have been demonstrated with  $\sim 30\,000$  degrees of freedom – and in the case of FF-GS, with twice the number of free parameters to estimate the pupil amplitudes.

The sampling at the detector was such that the controlled wavefront of  $170 \times 170$  pixels would have been enough to correct all spatial frequencies inside an image of  $640 \times 640$  pixels. However, as we recorded only an image of  $320 \times 320$  pixels, we had no direct observations of the higher controlled spatial frequencies. Simulations indicate that this resulted in a small amount of light being scattered outside the recorded field, but this amount was too small to be easily detected in our optical setup.

We put no particular effort into optimizing the codes; all the software was implemented in Matlab, and it was run on a standard Windows PC. Still, the required computation time was negligible compared to the time of  $\sim 15$  s we needed to collect data for a single HDR image. We implemented the FF algorithm with two  $640 \times 640$  FFTs per iteration step (one FFT transferring the phase-diversity information into the focal plane could likely be replaced by a convolution, as explained in [13]). Our FF-GS implementation used 8 FFTs per iteration, and that could also potentially be optimized.

As with all focal-plane wavefront sensing techniques, the algorithms work best if a monochromatic light source is available. With a chromatic light source having a sufficiently small bandwidth, perhaps  $\sim 10\%$ , the algorithms would still work, but

only with a limited corrected field. With special chromatic optics (such as in [19]) or an integral field unit, it is potentially possible to use the algorithms with even wider bandwidth.

Currently, we have only demonstrated a case where an unobstructed PSF is detected, and the wavefront is driven to be flat. To make the algorithms more interesting for astronomical applications in the extreme adaptive optics or ultra-high contrast imaging, a few extensions would be necessary.

First, we should consider how coronagraphs and diffraction suppression optics will affect the techniques. In practice, this would mean that the core of the PSF would not be detected, and we would need to consider also the moduli in a part of the focal-plane field as free parameters.

Second, instead of flattening the wavefront, we should optimize the contrast at a certain part of the field. This would mean calculating a wavefront shape that, in the same way as in [9, 20, 21], minimizes the light in certain regions of the field at the cost of increasing it in other parts; the updated algorithm should then drive the wavefront to this desired shape. A similar problem is faced, if phase plates are used to create diffraction suppression, for instance as in [22]. Also in such a case, it is necessary to drive the wavefront to a particular shape that is far from flat.

Another, potentially interesting application is a real-time application, for instance as a high-order, second-stage sensor in an adaptive optics system. The computational load is manageable, and a successful system would greatly simplify the hardware design compared to a conventional AO approach. However, issues such as the requirement for small aberrations, chromaticity, temporal lag in the phase diversity and the limited dynamic range of the camera – and therefore photon noise – are major challenges.

## References

- [1] R. W. Gerchberg and W. O. Saxton, “A practical algorithm for the determination of the phase from image and diffraction plane pictures,” *Optik* **35**, 237–246 (1972).
- [2] J. R. Fienup, “Phase retrieval algorithms: a comparison,” *Applied Optics* **21**, 2758–2769 (1982).
- [3] J. J. Green, D. C. Redding, S. B. Shaklan, and S. A. Basinger, “Extreme wave front sensing accuracy for the Eclipse coronagraphic space telescope,” in “High-Contrast Imaging for Exo-Planet Detection,” , vol. 4860 of *Proc. SPIE*, A. B. Schultz, ed. (2003), vol. 4860 of *Proc. SPIE*, pp. 266–276.

- [4] R. S. Burruss, E. Serabyn, D. P. Mawet, J. E. Roberts, J. P. Hickey, K. Rykoski, S. Bikkannavar, and J. R. Crepp, “Demonstration of on sky contrast improvement using the modified Gerchberg-Saxton algorithm at the Palomar Observatory,” (2010), vol. 7736 of *Proc. SPIE*.
- [5] J. Sauvage, T. Fusco, G. Rousset, and C. Petit, “Calibration and precompensation of noncommon path aberrations for extreme adaptive optics,” *J. Opt. Soc. Am. A* **24**, 2334–2346 (2007).
- [6] P. Riaud, D. Mawet, and A. Magette, “Nijboer-Zernike phase retrieval for high contrast imaging. Principle, on-sky demonstration with NACO, and perspectives in vector vortex coronagraphy,” *Astron. Astrophys.* **545**, A150 (2012).
- [7] B. Paul, L. M. Mugnier, J.-F. Sauvage, M. Ferrari, and K. Dohlen, “High-order myopic coronagraphic phase diversity (COFFEE) for wave-front control in high-contrast imaging systems,” *Optics Express* **21**, 31751 (2013).
- [8] C. Véraud, M. Kasper, J.-L. Beuzit, R. G. Gratton, D. Mesa, E. Aller-Carpentier, E. Fedrigo, L. Abe, P. Baudoz, A. Boccaletti, M. Bonavita, K. Dohlen, N. Hubin, F. Kerber, V. Korkiakoski, J. Antichi, P. Martinez, P. Rabou, R. Roelfsema, H. M. Schmid, N. Thatte, G. Salter, M. Tecza, L. Venema, H. Hanenburg, R. Jager, N. Yaitskova, O. Preis, M. Orecchia, and E. Stadler, “System study of EPICS: the exoplanets imager for the E-ELT,” in “Adaptive Optics Systems II,” , vol. 7736 of *Proc. SPIE* (2010), vol. 7736 of *Proc. SPIE*, pp. 77361N–77361N–12.
- [9] A. Give’On, R. Belikov, S. Shaklan, and J. Kasdin, “Closed loop, DM diversity-based, wavefront correction algorithm for high contrast imaging systems,” *Opt. Express* **15**, 12338 (2007).
- [10] C. S. Smith, R. Marinică, A. J. den Dekker, M. Verhaegen, V. Korkiakoski, C. U. Keller, and N. Doelman, “Iterative linear focal-plane wavefront correction,” *Journal of the Optical Society of America A* **30**, 2002 (2013).
- [11] S. Meimon, T. Fusco, and L. M. Mugnier, “Lift: a focal-plane wavefront sensor for real-time low-order sensing on faint sources,” *Opt. Lett.* **35**, 3036–3038 (2010).
- [12] F. Martinache, “The Asymmetric Pupil Fourier Wavefront Sensor,” *Publ. Astron. Soc. Pac.* **125**, 422–430 (2013).
- [13] C. U. Keller, V. Korkiakoski, N. Doelman, R. Fraanje, R. Andrei, and M. Verhaegen, “Extremely fast focal-plane wavefront sensing for extreme adaptive optics,” (2012), vol. 8447 of *Proc. SPIE*, pp. 844721–844721.
- [14] V. Korkiakoski, C. U. Keller, N. Doelman, R. Fraanje, R. Andrei, and M. Verhaegen, “Experimental validation of optimization concepts for focal-plane image processing with adaptive optics,” (2012), vol. 8447 of *Proc. SPIE*, pp. 84475Z–84475Z.
- [15] V. Korkiakoski, N. Doelman, J. Codona, M. Kenworthy, G. Otten, and C. U. Keller, “Calibrating a high-resolution wavefront corrector with a static focal-plane camera,” *Appl. Opt.* **52**, 7554 (2013).
- [16] R. A. Gonsalves, “Small-phase solution to the phase-retrieval problem,” *Optics Letters* **26**, 684–685 (2001).
- [17] M. D. Perrin, A. Sivaramakrishnan, R. B. Makidon, B. R. Oppenheimer, and J. R. Graham, “The Structure of High Strehl Ratio Point-Spread Functions,” *Astrophys. J.* **596**, 702–712 (2003).
- [18] L. C. Roberts, Jr., M. D. Perrin, F. Marchis, A. Sivaramakrishnan, R. B. Makidon, J. C. Christou, B. A. Macintosh, L. A. Poyneer, M. A. van Dam, and M. Troy, “Is that really your Strehl ratio?” in “Advancements in Adaptive Optics,” , vol. 5490 of *Proc. SPIE* (2004), vol. 5490 of *Proc. SPIE*, pp. 504–515.
- [19] O. Guyon, “High Sensitivity Wavefront Sensing with a Nonlinear Curvature Wavefront Sensor,” *Publ. Astron. Soc. Pac.* **122**, 49–62 (2010).
- [20] F. Malbet, J. W. Yu, and M. Shao, “High-Dynamic-Range Imaging Using a Deformable Mirror for Space Coronagraphy,” *Publ. Astron. Soc. Pac.* **107**, 386 (1995).
- [21] P. J. Bordé and W. A. Traub, “High-Contrast Imaging from Space: Speckle Nulling in a Low-Aberration Regime,” *Astrophys. J.* **638**, 488–498 (2006).
- [22] J. L. Codona and R. Angel, “Imaging Extrasolar Planets by Stellar Halo Suppression in Separately Corrected Color Bands,” *The Astrophysical Journal Letters* **604**, L117–L120 (2004).