# HYADES MEMBER K2-136c: THE SMALLEST PLANET IN AN OPEN CLUSTER WITH A PRECISELY MEASURED MASS

Andrew W. Mayo<sup>1,2,†,‡</sup>, Courtney D. Dressing<sup>1</sup>, Andrew Vanderburg<sup>3</sup>, Charles D. Fortenbach<sup>4</sup>, Florian Lienhard<sup>5</sup>, Luca Malavolta<sup>7</sup>, Annelies Mortier<sup>5,6,8</sup>, Alejandro Núñez<sup>10</sup>, Tyler Richey-Yowell<sup>11</sup>, Emma V. Turtelboom<sup>1</sup>, Aldo S. Bonomo<sup>12</sup>, David W. Latham<sup>13</sup>, Mercedes López-Morales<sup>13</sup>, Evgenya Shkolnik<sup>11</sup>, Alessandro Sozzetti<sup>12</sup>, Marcel A. Agüeros<sup>9,10</sup>, Luca Borsato<sup>14</sup>, David Charbonneau<sup>13</sup>, Rosario Cosentino<sup>15</sup>, Stephanie T. Douglas<sup>16</sup>, Xavier Dumusque<sup>17</sup>, Adriano Ghedina<sup>15</sup>, Rose Gibson<sup>18</sup>, Valentina Granata<sup>7,14</sup>, Avet Harutyunyan<sup>15</sup>, R. D. Haywood<sup>19</sup>, Gaia Lacedelli<sup>7,14</sup>, Vania Lorenzi<sup>15,20</sup>, Antonio Magazzù<sup>15</sup>, A. F. Martinez Fiorenzano<sup>15</sup>, Giuseppina Micela<sup>21</sup>, Emilio Molinari<sup>22</sup>, Marco Montalto<sup>7</sup>, Domenico Nardiello<sup>23,14</sup>, Valerio Nascimbeni<sup>14</sup>, Isabella Pagano<sup>24</sup>, Giampaolo Piotto<sup>7,14</sup>, Lorenzo Pino<sup>25</sup>, Ennio Poretti<sup>15,26</sup>, Gaetano Scandariato<sup>23</sup>, Stephane Udry<sup>16</sup>, Lars A. Buchhave<sup>2,27</sup>

Draft version April 7, 2023

## ABSTRACT

K2-136 is a late-K dwarf  $(0.742 \pm 0.039 \text{ M}_{\odot})$  in the Hyades open cluster with three known, transiting planets and an age of  $650 \pm 70$  Myr. Analyzing K2 photometry, we found that planets K2-136b, c, and d have periods of 8.0, 17.3, and 25.6 days and radii of  $1.014 \pm 0.050$  R<sub> $\oplus$ </sub>,  $3.00 \pm 0.13$  R<sub> $\oplus$ </sub>, and  $1.565 \pm 0.077$  R<sub> $\oplus$ </sub>, respectively. We collected 93 radial velocity measurements (RVs) with the HARPS-N spectrograph (TNG) and 22 RVs with the ESPRESSO spectrograph (VLT). Analyzing HARPS-N and ESPRESSO data jointly, we found K2-136c induced a semi-amplitude of  $5.49 \pm 0.53$ m s<sup>-1</sup>, corresponding to a mass of  $18.1 \pm 1.9$  M<sub> $\oplus$ </sub>. We also placed 95% upper mass limits on K2-136b and d of 4.3 and 3.0  $M_{\oplus}$ , respectively. Further, we analyzed HST and XMM-Newton observations to establish the planetary high-energy environment and investigate possible atmospheric loss. K2-136c is now the smallest planet to have a measured mass in an open cluster and one of the youngest planets ever with a mass measurement. K2-136c has  $\sim 75\%$  the radius of Neptune but is similar in mass, yielding a density of  $3.69^{+0.67}_{-0.56}$  g cm<sup>-3</sup> ( $\sim$ 2-3 times denser than Neptune). Mass estimates for K2-136b (and possibly d) may be feasible with more RV observations, and insights into all three planets' atmospheres through transmission spectroscopy would be challenging but potentially fruitful. This research and future mass measurements of young planets are critical for investigating the compositions and characteristics of small exoplanets at very early stages of their lives and providing insights into how exoplanets evolve with time.

Keywords: planets and satellites: composition - planets and satellites: detection - planets and satellites: fundamental parameters - planets and satellites: rocky planets - methods: data analysis techniques: radial velocities

# † mayo@berkeley.edu

- <sup>‡</sup> National Science Foundation Graduate Research Fellow
- <sup>1</sup> Astronomy Department, University of California, Berkeley,
- Centre for Star and Planet Formation, Natural History Museum of Denmark & Niels Bohr Institute, University of Copenhagen, Øster Voldgade 5-7, DK-1350 Copenhagen K., Denmark

Department of Physics and Kavli Institute for Astrophysics and Space Research, Massachusetts Institute of Technology, 77 Massachusetts Avenue, Cambridge, MA, 02139, USA

<sup>4</sup> Department of Physics and Astronomy, San Francisco State University, San Francisco, CA 94132, USA

<sup>5</sup> Astrophysics Group, Cavendish Laboratory, University of

- Cambridge, J. J. Thomson Avenue, Cambridge CB3 0HE, UK <sup>6</sup> School of Physics & Astronomy, University of Birmingham, Edgbaston, Birmingham, B15 2TT, UK
- Dipartimento di Fisica e Astronomia Galileo Galilei, Universitá di Padova, Vicolo dell'Osservatorio 3, 35122 Padova, Italy 8 Kavli Institute for Cosmology, University of Cambridge, Madingley Road, Cambridge CB3 0HA, UK

<sup>9</sup> Laboratoire d'astrophysique de Bordeaux, Univ. Bordeaux, CNRS, B18N, Allée Geoffroy Saint-Hilaire, 33615 Pessac, France

10 Department of Astronomy, Columbia University, 550 West 120th Street, New York, NY 10027, USA

11 School of Earth and Space Exploration, Arizona State Uni-

versity, Tempe, AZ 85287, USA

12 INAF – Osservatorio Astrofisico di Torino, Via Osservato-

rio 20, 10025 Pino Torinese, Italy <sup>13</sup> Center for Astrophysics | Harvard & Smithsonian, 60 Garden Street, Cambridge, MA 02138, USA

- $^{14}\,\mathrm{INAF}$  Osservatorio Astronomico di Padova, Vicolo dell'Osservatorio 5, IT-35122, Padova, Italy
- <sup>15</sup> Fundación Galileo Galilei-INAF, Rambla José Ana Fernandez Pérez 7, 38712 Breña Baja, Tenerife, Spain
- <sup>16</sup> Department of Physics, Lafayette College, 730 High Street, Easton, PA 18042, USA
- <sup>17</sup> Department of Astronomy of the University of Geneva, Geneva Observatory, Chemin Pegasi 51, 1290 Versoix, Switzer-
- <sup>18</sup> Columbia University, Department of Astronomy, 550 West 120th Street, New York, USA, 10027
- <sup>19</sup> Astrophysics Group, University of Exeter, Exeter EX4 2QL,
- UK 20 Instituto de Astrofísica de Canarias, C/Vía Láctea s/n, 38205La Laguna, Spain $^{21}\,\mathrm{INAF}$ - Osservatorio Astronomico di Palermo, Piazza del
- Parlamento 1, I-90134 Palermo, Italy
- <sup>22</sup> INAF Osservatorio Astronomico di Cagliari & REM, Via della Scienza, 5, 09047 Selargius CA, Italy
- Aix Marseille Univ, CNRS, CNES, LAM, Marseille, France <sup>24</sup> INAF – Osservatorio Astrofisico di Catania, Via Santa Sofia 78, 95123 Catania, Italy  $^{\rm 25}$  INAF - Osservatorio Astrofisico di Arcetri, Largo Enrico
- Fermi 5, 50125, Firenze, Italy
- <sup>26</sup> INAF Osservatorio Astronomico di Brera, Via E. Bianchi 46, 23807 Merate, Italy <sup>27</sup> DTU Space, National Space Institute, Technical University
- of Denmark, Elektrovej 327, DK-2800 Lyngby, Denmark

## 1. INTRODUCTION

The timescales on which planets and planetary systems evolve are far longer than any feasible timescale of scientific observations. The only way to learn about how planets form and evolve is to collect snapshots at different stages of their development and assemble these snapshots into a cohesive framework. This is where open clusters prove particularly useful. Open clusters, close collections of young, recently formed stars, are excellent laboratories for studying the early lives of stars, because all of the stars in an open cluster, regardless of size, temperature, metallicity, or location, have a shared formation history, and therefore the ages of the stars can be very tightly constrained. This logic can also be applied to planets; if they form very quickly after the coalescence of their host star (Raymond & Morbidelli 2020), it is possible to determine the age of a planet orbiting an open cluster star, thereby capturing one of the early snapshots required to assemble the framework of a planet's evolution.

In this paper we characterize K2-136c, a sub-Neptune planet in the Hyades open cluster. Orbiting a late K dwarf, this planet is one of the three known, transiting planets in the system. The system was originally observed in K2 Campaign 13 for 80 days (2017 March 8-2017 May 27) and was proposed for observation by seven guest observer teams: GO13008, GO13018, GO13023, GO13049, GO13064, GO13077, and GO13090. All three planets were originally discovered by Mann et al. (2018) (hereafter M18) and Ciardi et al. (2018) (a parallel analysis published simultaneously). Shortly thereafter a subsequent analysis was completed by Livingston et al. (2018). All three papers are in broad agreement regarding stellar and planetary parameters, but M18 established the tightest constraints on orbital period for all three planets.

In their analysis, M18 found an Earth-sized planet  $(0.99^{+0.06}_{-0.04}~\rm R_{\oplus})$  at P=8.0 days (K2-136b), a sub-Neptune-sized planet  $(2.91^{+0.11}_{-0.10}~\rm R_{\oplus})$  at P=17.3 days (K2-136c, the focus of this paper), and a super-Earth-sized planet  $(1.45^{+0.11}_{-0.08}~\rm R_{\oplus})$  at P=25.6 days (K2-136d). They also determined a host star mass of  $0.74\pm0.02~\rm M_{\odot}$  and a stellar radius of  $0.66\pm0.02~\rm R_{\odot}$ .

As for the stellar age, there are a number of estimates available. Perryman et al. (1998) found the Hyades open cluster to be  $625 \pm 50$  Myr. Gossage et al. (2018) found an age of  $\sim 680$  Myr while Brandt & Huang (2015) determined a slightly older age of  $750 \pm 100$  Myr. The age we use throughout this paper comes from Martín et al. (2018), who determined the Hyades to be  $650 \pm 70$  Myr old. We thus assume that K2-136 and the three orbiting planets share that approximate age. We chose this age because it is a relatively recent result, it compares and combines results using both old (Burrows et al. 1997) and new (Baraffe et al. 2015) standard evolutionary models, and it also agrees broadly with other, previous estimates. The young age of the system was our primary reason for pursuing K2-136c as a target: there are very few young, small planets with mass measurements. According to the NASA Exoplanet Archive (accessed 2023 Mar 12; NASA Exoplanet Science Institute 2020), there are only 13 confirmed exoplanets with  $R_p < 4 \text{ R}_{\oplus}$ , a host star age < 1 Gyr, and a mass measurement (not an upper limit): HD 18599b (Desidera et al. 2022), HD 73583b and c (Barragán et al. 2022); K2-25b (Stefansson et al. 2020); L 98-59b, c, and d (Demangeon et al. 2021); Kepler-411b and Kepler-411d (Sun et al. 2019); Kepler-462b (Masuda & Tamayo 2020); Kepler-289b and Kepler-289d (Schmitt et al. 2014); and K2-100b (Barragán et al. 2019). Of these, only the Kepler-411, K2-100, HD 73583, K2-25, and HD 18599 systems have an age constraint tighter than 50% (Sun et al. 2019; Barragán et al. 2019, 2022; Stefansson et al. 2020; Desidera et al. 2022).

We analyzed photometry of the K2-136 system in order to measure the radii, ephemerides, and other transit parameters of each planet. We also collected spectra of the K2-136 system and measured radial velocities (RVs) as well as stellar activity indices. Then, by modeling these RVs (following Rajpaul et al. 2015), we determined the mass of K2-136c and placed upper limits on the masses of the other two planets. We used this system to investigate the nature, environment, and evolution of young, small exoplanets.

This paper is organized as follows. In Section 2 we discuss our observations. Then we detail our method of stellar characterization in Section 3. Next, in Section 4 we describe our RV and photometry models, data analysis, model comparison, and parameter estimation. In Section 5 we present and discuss our results. Finally, we summarize and conclude in Section 6.

#### 2. OBSERVATIONS

#### 2.1. K2

Photometric observations of the K2-136 system were collected with the Kepler spacecraft (Borucki et al. 2008) through the K2 mission during Campaign 13 (2017 Mar 08 to 2017 May 27). K2 collected long-cadence observations of this system every 29.4 minutes.

# 2.2. TESS

Photometric observations of the K2-136 system were also collected with the TESS spacecraft (Ricker et al. 2015) during Sector 43 (2021 Sep 16 to 2021 Oct 10) and Sector 44 (2021 Oct 12 to 2021 Nov 06). TESS collected long-cadence full frame image observations of this system every 10 minutes in Sector 43 and short-cadence observations every 20 seconds in Sector 44.

## 2.3. HARPS-N

We collected 93 RV observations using the HARPS-N spectrograph (Cosentino et al. 2012, Cosentino et al. 2014) on the Telescopio Nazionale Galileo (TNG). The first 88 spectra were collected between 2018 August 11 and 2019 February 7 (programs A37TAC\_24 and A38TAC\_27, PI: Mayo), and the final 5 spectra were collected between 2020 September 18 and 2020 October 31 by the HARPS-N Guaranteed Time Observation program. RVs and additional stellar activity indices were extracted using a K6 stellar mask and version 2.2.8 of the Data Reduction Software (DRS) adapted from the ESPRESSO pipeline. Spectra had an average exposure time of 1776.5 seconds and the average SNR in the order around 550 nm was 51.1. The RV standard deviation was  $6.9 \text{ m s}^{-1}$  and the RV median uncertainty was  $1.6 \text{ m s}^{-1}$ . Stellar activity indices also extracted and reported in this paper include the cross-correlation function (CCF) bisector span inverse slope (hereafter BIS), the CCF full width

at half maximum (FWHM), and  $S_{HK}$  (which measures chromospheric activity via core emission in the Ca II H and K absorption lines). The observation dates, velocities, and activity indices are provided in Table 2.

## 2.4. ESPRESSO

We collected 22 RV observations using the ESPRESSO spectrograph (Pepe et al. 2021) on the Very Large Telescope (VLT) between 2019 November 1 and 2020 February 27 (program 0104.C-0837(A), PI: Malavolta). RVs and additional stellar activity indices were extracted using a K6 stellar mask and the same pipeline as the HARPS-N observations (DRS version 2.2.8). Typical exposure time for spectra was 1800 seconds and the average SNR at Order 111 (central wavelength = 551nm) was 79.9. The RV standard deviation was 7.8 m s $^{-1}$  and the RV median uncertainty was 0.70 m s $^{-1}$ . These observations and indices are also provided in Table 2.

# 2.5. Hubble Space Telescope

Near-ultraviolet (NUV) observations of K2-136 were taken as part of a broader *Hubble Space Telescope* (*HST*) program observing the Hyades (GO-15091, PI: Agüeros). The target was exposed for 1166.88 seconds on 2019 September 13 using the photon-counting Cosmic Origins Spectrograph (COS; Green et al. 2012) in the G230L filter and had no data quality flags.

After initial data reduction through the CALCOS pipeline version 3.3.10, we additionally confirmed that the star was not flaring during observations by integrating the background-subtracted flux by wavelength over 1 and 10 second time intervals in the time-tagged data. No flares above  $3\sigma$  were identified.

# 2.6. XMM-Newton

K2-136 was the target of an XMM-Newton (XMM) 43 ksec observation on 2018 September 11 (Obs. ID: 0824850201, PI: Wheatley). The observation was processed using the standard Pipeline Processing System (PPS version 17.56\_20190403\_1200; Pipeline sequence ID: 147121). The source detection corresponding to K2-136 was detected by both the pn and MOS cameras, for a total of 800 source counts in the 0.2-12.0 keV energy band. The X-ray source has data quality flag SUM\_FLAG=0 (i.e., good quality). No variability or pileup were detected for this X-ray source.

## 3. STELLAR CHARACTERIZATION

In order to characterize the star, we started by combining all of our collected HARPS-N spectra (from 2018-2019) into a single, stacked spectrum with S/N  $\sim 300$  (based on signal divided by scatter on continuum segments near 6000 Å; see Section 3.1 of Mortier et al. 2013 for more details). Then we ran the ARESv2 package (Sousa et al. 2015) to obtain equivalent widths for a standard set of neutral and ionised iron lines (Sousa et al. 2011). We refer to Mortier et al. (2013), Sousa (2014), and Sousa et al. (2015) for our choice of typical model parameters. Afterward, we calculated stellar parameters using MOOG¹ (Sneden 1973) with ATLAS

plane-parallel model atmospheres (Kurucz 1993) assuming local thermodynamic equilibrium. A downhill simplex minimization procedure (Press et al. 1992) was used to determine the stellar photospheric parameters (see e.g. Mortier et al. 2013, and references therein). We determined that the stellar temperature was less than 5200 K, so we reran the minimization procedure with a sublist of lines designed for cooler stars (Tsantaki et al. 2013); we also constrained our line list to those with equivalent widths between 5 and 150 milliAngstroms (mÅ), removing 5 lines above 150 mÅ and 1 line below 5 mÅ (lines within this range tend to be sufficiently strong and well-described by a Gaussian). Finally, we corrected for  $\log g$  and re-scaled errors following Torres et al. (2012), Mortier et al. (2014), and Sousa et al. (2011). The resulting effective temperature, surface gravity, microturbulence, and metallicity are reported in Table 1.

Then we determined the same stellar parameters from the same spectra with a different, independent tool: the Stellar Parameter Classification tool (SPC; Buchhave et al. 2012). SPC interpolates across a synthetic spectrum library from Kurucz (1992) to find the best fit and uncertainties on an input spectrum. In addition to the stellar parameters calculated from ARES+MOOG, this tool also estimated rotational velocity. All atmospheric stellar parameters from ARES+MOOG and SPC were in good agreement (within  $1\sigma$ ). Like ARES+MOOG, all SPC parameter estimates can be found in Table 1.

We then took our estimated effective temperature and metallicity from ARES+MOOG and SPC, the Gaia Data Release 3 (DR3) parallax (Gaia Collaboration et al. 2016. 2020; Gaia Collaboration & Vallenari 2022), and numerous photometric magnitudes (B, V, J, H, K, W1, W2, and W3) and input them into the isochrones Python package (Morton 2015). This package used two different sets of isochrones: Dartmouth (Dotter et al. 2008) and Modules for Experiments in Stellar Astrophysics (MESA) Isochrones and Stellar Tracks (MIST; Choi et al. 2016; Dotter 2016). Comparing two standard, independent models is useful for mitigating systematic errors and revealing discrepancies or issues in the resulting parameter estimates. We used MultiNest (Feroz et al. 2009, 2013) for parameter estimation, assuming 600 live points and otherwise standard MultiNest settings: importance nested sampling mode, multimodal mode, constant efficiency mode disabled, evidence tolerance = 0.5, and sampling efficiency = 0.8. As stated earlier, K2-136 is a member of the Hyades and therefore has a very tight age constraint of  $650 \pm 70$  Myr (Martín et al. 2018). We applied a much broader age prior of 475 Myr - 775 Myr (a  $3\sigma$  range on the  $625 \pm 50$  Hyades age estimate from Perryman et al. 1998), which was more than sufficient to achieve convergence. This yielded posterior distributions from both input atmospheric parameter sets (ARES+MOOG and SPC) as well as both isochrone sets (Dartmouth and MIST), for a total of four sets of posterior distributions (based on all combinations of input parameters and isochrones).

The posteriors were then combined together (i.e. the posterior samples were appended together) to yield a single posterior distribution for each parameter. Lastly, systematic uncertainties determined by Tayar et al. (2020) were added in quadrature to the combined posteriors to

 $<sup>^1</sup>$  2017 version: <code>http://www.as.utexas.edu/\$\sim\$chris/moog.html</code>

Table 1 Stellar parameters of K2-136

Parameter	Unit			Value	Reference
EPIC				247589423	
2MASS	_		•••••	J04293897+2252579	-
$\alpha$ R.A.	J2016.0			04:29:39.1	GAIA DR3 <sup>a</sup>
$\delta$ Dec	J2016.0			+22.52.57.2	GAIA DR3
$\mu_{\alpha}$	$mas yr^{-1}$			$82.778 \pm 0.021$	GAIA DR3a
$\mu_{\delta}$	$\mathrm{mas\ yr}^{-1}$			$-35.541 \pm 0.015$	GAIA DR3 <sup>a</sup>
Parallax	mas			$16.982 \pm 0.019$	GAIA DR3 <sup>a</sup>
Distance	pc			$58.752^{+0.061}_{-0.072}$	b
Age	Myr			$650 \pm 70^{-2}$	c
B mag	-			$12.48 \pm 0.01$	$\rm UCAC4^{d}$
V mag	-			$11.20 \pm 0.01$	$UCAC4^{d}$
J mag	-			$9.096 \pm 0.022$	$2MASS^e$
H mag	-			$8.496 \pm 0.020$	$2MASS^e$
K mag	-			$8.368 \pm 0.019$	$2MASS^e$
W1 mag	-			$8.263 \pm 0.023$	$\mathrm{WISE^f}$
W2 mag				$8.349 \pm 0.020$	$\mathrm{WISE}^{\mathrm{f}}$
W3 mag				$8.312 \pm 0.030$	$\mathrm{WISE}^{\mathrm{f}}$
Fractional X-ray luminosity $L_{\rm X}/L_{*}$	-			$(1.97 \pm 0.30) \times 10^{-5}$	This work
Parameter	Unit	SPC	ARES+MOOG	Combined <sup>g</sup>	Reference
				1.105	
Effective temperature $T_{\rm eff}$	K	$4517 \pm 49$	$4447 \pm 149$	$4500^{+125}_{-75}$	This work
Surface gravity $\log g$	${ m g~cm^{-2}}$	$4.68 \pm 0.10$	$4.82 \pm 0.43$	-	This work
Microturbulence	${ m km~s^{-1}}$	-	$< 1.1^{\rm h}$	-	This work
Metallicity [Fe/H]	dex	-	$0.05 \pm 0.10$	-	This work
Metallicity [M/H]	dex	$-0.02 \pm 0.08$	-	-	This work
Radius $R_*$	${ m R}_{\odot}$	$0.6764^{+0.0039}_{-0.0033}$	$0.6770^{+0.0050}_{-0.0038}$	$0.677 \pm 0.027$	This work
Mass $M_*$	$ m M_{\odot}$	$0.7413^{+0.0093}_{-0.0056}$	$0.7430^{+0.0126}_{-0.0070}$	$0.742^{+0.039}_{-0.038}$	This work
Density $\rho_*$	$ ho_{\odot}$	$2.397^{+0.017}$	$2.397^{+0.018}_{-0.010}$	$2.40 \pm 0.31$	This work
Luminosity $L_*$	$ m L_{\odot}$	$0.1682^{+0.0043}_{-0.0035}$	0.1664 + 0.0038	$0.1673^{+0.0053}_{-0.0049}$	This work
Projected rot. velocity $v \sin i$	${ m km~s^{-1}}$	< 2	0.1004_0.0035	-0.0049	This work
1 To jectica 100. Velocity to Sill t	MIII D				THIS WOLK

<sup>&</sup>lt;sup>a</sup>Gaia Collaboration et al. (2016, 2020); Babusiaux et al. (2022); Gaia Collaboration & Vallenari (2022)

yield final parameters and uncertainties. Specifically, we added 4% uncertainty to  $R_{\odot}$ , 5% uncertainty to  $M_{\odot}$ , 2% uncertainty to  $L_{\odot}$ , and 13% uncertainty to  $\rho_{\odot}$  (propagated from  $R_{\odot}$  and  $M_{\odot}$  uncertainties). The input GaiaDR3 parallax, distance, photometric magnitudes, and the resulting stellar radius, mass, density, and luminosity are all reported in Table 1.

Table 2 RV observations and activity indicators

BJD (TDB)	RV	$\sigma_{ m RV}$	CCF BIS	$\sigma_{ m BIS}$	CCF FWHM	$\sigma_{ m FWHM}$	$S_{HK}$	$\sigma_{ m S_{HK}}$	Instrument
` ,	$(m \ s^{-1})$	$(m s^{-1})$	$(m s^{-1})$	$(m s^{-1})$	$(m s^{-1})$	$(m s^{-1})$		1110	
-	( )	( )	( )	( )	( )	( )			
2458341.70618026	39498.9	1.8	6901.1	3.7	63.8	3.7	1.191	0.022	HARPS-N
2458345.70159539	39516.8	1.4	6920.6	2.7	63.4	2.7	1.198	0.014	HARPS-N
2458346.70175761	39515.5	2.0	6948.0	4.0	70.2	4.0	1.274	0.025	HARPS-N
2458361.71645940	39513.6	2.9	6945.1	5.7	75.3	5.7	1.234	0.039	HARPS-N
2458363.75019615	39514.0	1.4	6942.8	2.8	69.2	2.8	1.222	0.013	HARPS-N
2458364.69673319	39516.3	1.4	6941.9	2.8	74.6	2.8	1.251	0.014	HARPS-N
2458365.69775405	39515.1	1.3	6949.1	2.7	71.9	2.7	1.238	0.013	HARPS-N
2458366.72988568	39504.4	1.7	6932.3	3.3	83.8	3.3	1.212	0.018	HARPS-N
2458378.65078445	39517.9	2.2	6947.9	4.4	72.8	4.4	1.294	0.027	HARPS-N
2458379.66372361	39514.4	1.4	6945.1	2.8	80.4	2.8	1.249	0.014	HARPS-N
2458380.65930503	39510.6	1.2	6930.6	2.4	77.3	2.4	1.294	0.012	HARPS-N
2458381.66442355	39504.7	1.2	6921.7	2.3	86.1	2.3	1.251	0.011	HARPS-N
2458382.66425283	39501.7	1.6	6913.0	3.2	78.8	3.2	1.243	0.018	HARPS-N
2458383.66210025	39495.8	2.3	6902.9	4.5	75.2	4.5	1.172	0.029	HARPS-N
2458384.71464839	39498.4	2.2	6896.4	4.4	67.9	4.4	1.160	0.027	HARPS-N
2458385.66982781	39500.0	1.4	6900.7	2.8	63.5	2.8	1.162	0.014	HARPS-N

<sup>&</sup>lt;sup>b</sup>Bailer-Jones et al. (2021)

<sup>&</sup>lt;sup>c</sup>Martín et al. (2018)

dZacharias et al. (2013) Cutri et al. (2003); Skrutskie et al. (2006)

fWright et al. (2010)

gSystematic uncertainties added in quadrature (Tayar et al. 2020)

 $<sup>^{\</sup>rm h}{\rm Value}$  is poorly constrained,  $1\sigma$  upper limit reported instead

Table 2 (continued)
RV observations and activity indicators

BJD (TDB)										
2468861,7771712   300001   1.5   6010.7   2.1   50.8   2.1   1.105   60.101   HARPS-N   2468803,75391115   30507.6   1.5   6022.3   3.0   60.3   2.0   1.1194   60.101   HARPS-N   2468801,75391115   30507.6   1.5   6023.3   3.0   60.3   2.0   1.1194   60.101   HARPS-N   2468810,64445231   3509.0   1.5   607674   2.9   65.3   2.9   1.203   60.115   HARPS-N   2458410,64445231   3509.0   2.7   609.1   2.4   609.2   5.4   81.5   5.4   1.143   0.037   HARPS-N   2458410,64445231   3509.0   2.7   609.1   5.4   60.6   6.7   4.8   1.130   60.028   HARPS-N   2458410,7451711   33506.0   2.7   609.1   4.8   66.7   4.8   1.130   60.028   HARPS-N   2458412,72295116   309.07   2.4   600.5   4.8   66.7   4.8   1.130   60.028   HARPS-N   2458412,72295116   309.07   4.4   602.2   8.8   6.7   4.8   1.130   60.028   HARPS-N   2458412,72295116   309.07   4.4   602.2   8.8   6.7   4.8   8.1   1.3   6.0   6.7   4.8	BJD (TDB)	RV	$\sigma_{\text{RV}}$	CCF BIS	$\sigma_{\mathrm{BIS}}$	CCF FWHM	$\sigma_{\text{FWHM}}$	$S_{HK}$	$\sigma_{ m S_{HK}}$	Instrument
245888,70001017 39504.0 1.4 6916.2 2.9 02.5 2.9 1.213 0.015 HARPS-N 245880,739115 39507.6 1.5 0623.3 3.0 0.63 3.0 1.194 0.016 HARPS-N 245881,74332111 39509.3 1.5 6907.4 2.9 65.3 2.9 1.203 0.015 HARPS-N 245811,74332111 39509.3 1.5 6907.4 2.9 65.3 2.9 1.203 0.015 HARPS-N 245811,7433211 39509.3 1.5 6907.4 2.9 68.7 2.9 1.503 0.015 HARPS-N 245811,51383839 39507.7 2.4 6906.6 4.8 66.5 4.8 1.130 0.028 HARPS-N 245811,51383839 39507.7 2.4 6906.6 4.8 66.5 4.8 1.130 0.028 HARPS-N 2458415,7238341 39504.5 1.4 6916.4 2.9 68.7 2.9 1.163 0.015 HARPS-N 2458412,1225691 39497.8 1.4 6916.4 2.9 68.7 2.9 1.163 0.015 HARPS-N 2458412,1225691 39497.8 1.4 6916.4 2.9 68.7 2.9 1.163 0.015 HARPS-N 3458412,1225691 39497.8 1.4 6916.4 2.9 68.7 2.9 1.163 0.015 HARPS-N 3458412,12256925 39506.0 1.4 6937.6 2.8 74.8 2.8 1.240 0.014 HARPS-N 2458412,122562529 39506.0 1.2 6915.5 3.6 67.0 5.7 69.0 5.8 7.7 1.247 0.002 HARPS-N 34584418,732032 39518.1 5.9 6925 12 81 12 1.17 0.011 HARPS-N 34584418,732032 39518.1 5.9 6925 12 81 12 1.17 0.11 HARPS-N 3458451,0543612 39512 39512 39512 39518 39512 2 2.9 6916.1 5.9 6925 12 81 12 1.17 0.11 HARPS-N 3458451,0543612 39512		(m s <sup>-1</sup> )	(m s <sup>-1</sup> )	(m s <sup>-1</sup> )						
245888,70001017 39504.0 1.4 6916.2 2.9 02.5 2.9 1.213 0.015 HARPS-N 245880,739115 39507.6 1.5 0623.3 3.0 0.63 3.0 1.194 0.016 HARPS-N 245881,74332111 39509.3 1.5 6907.4 2.9 65.3 2.9 1.203 0.015 HARPS-N 245811,74332111 39509.3 1.5 6907.4 2.9 65.3 2.9 1.203 0.015 HARPS-N 245811,7433211 39509.3 1.5 6907.4 2.9 68.7 2.9 1.503 0.015 HARPS-N 245811,51383839 39507.7 2.4 6906.6 4.8 66.5 4.8 1.130 0.028 HARPS-N 245811,51383839 39507.7 2.4 6906.6 4.8 66.5 4.8 1.130 0.028 HARPS-N 2458415,7238341 39504.5 1.4 6916.4 2.9 68.7 2.9 1.163 0.015 HARPS-N 2458412,1225691 39497.8 1.4 6916.4 2.9 68.7 2.9 1.163 0.015 HARPS-N 2458412,1225691 39497.8 1.4 6916.4 2.9 68.7 2.9 1.163 0.015 HARPS-N 3458412,1225691 39497.8 1.4 6916.4 2.9 68.7 2.9 1.163 0.015 HARPS-N 3458412,12256925 39506.0 1.4 6937.6 2.8 74.8 2.8 1.240 0.014 HARPS-N 2458412,122562529 39506.0 1.2 6915.5 3.6 67.0 5.7 69.0 5.8 7.7 1.247 0.002 HARPS-N 34584418,732032 39518.1 5.9 6925 12 81 12 1.17 0.011 HARPS-N 34584418,732032 39518.1 5.9 6925 12 81 12 1.17 0.11 HARPS-N 3458451,0543612 39512 39512 39512 39518 39512 2 2.9 6916.1 5.9 6925 12 81 12 1.17 0.11 HARPS-N 3458451,0543612 39512	2450206 72771712	20400 1	1.5	6010.7	9 1	50.2	9 1	1 165	0.016	HADDON
2458891,75891115 39690.7 d. 1.5 6923.3 3.0 66.3 3.0 1.194 0.016 HARPS-N 245810.0414221 3950.3 1.5 6907.4 2.9 65.3 2.9 1.03 0.015 HARPS-N 245811.04144221 3950.0 1.2 2 600.3 1.4 68.6 5.5 4.8 1.1 1.05 0.027 HARPS-N 245811.04144221 3950.0 1.2 2 600.3 1.4 68.6 5.5 4.8 1.1 1.05 0.027 HARPS-N 245811.04144221 3950.0 1.4 693.6 4.8 66.5 4.8 1.1 1.0 0.022 HARPS-N 245811.0 613850.3 930.0 1.2 2 600.5 4.8 66.5 4.8 1.1 1.0 0.022 HARPS-N 245811.0 7.0 1.0 1.0 1.0 1.0 1.0 1.0 1.0 1.0 1.0 1										
245817,74334211 39509.3 1.5 6007.4 2.9 65.3 2.0 1.203 0.015 IMARPS-N 245810,73761710 39506.9 2.7 6001.2 5.4 8.15 5.4 1.143 0.037 IMARPS-N 245810,73761710 39506.9 2.7 6001.2 5.4 8.15 5.4 1.143 0.037 IMARPS-N 245810,73761710 39506.9 2.7 6001.2 5.4 8.15 5.4 1.143 0.037 IMARPS-N 2458121,729201 39497.5 2.4 6007.5 2.8 74.8 2.8 1.20 0.014 IMARPS-N 2458121,64508501 39500.0 1.4 6037.6 2.8 74.8 2.8 1.20 0.014 IMARPS-N 2458121,729201 39497.5 2.4 6037.6 2.8 74.8 2.8 1.20 0.014 IMARPS-N 2458121,729248 39502.2 2.9 605.8 8.8 67.1 8.0 1.317 0.002 IMARPS-N 2458124,729248 39502.2 2.9 6001.5 5.3 695.5 5.7 1.247 0.041 IMARPS-N 2458144,7120334 3950.0 1.4 6007.5 3.6 600.2 2.9 1.0 1.1 1.1 1.1 1.1 1.1 1.1 1.1 1.1 1.1										
24581416.04440231 39506.1 2.2 6960.3 4.3 82.2 4.3 1.165 0.027 HARPS-N 2458141.361380389 39507.7 2.4 6905.6 4.8 8.5 5.4 1.143 0.037 HARPS-N 2458141.361380389 39507.7 2.4 6905.6 4.8 6.5 4.8 1.130 0.028 HARPS-N 2458121.7229616 39507.7 2.4 6905.6 4.8 6.5 7.8 8.9 1.30 0.0028 HARPS-N 2458121.7229616 39507.2 4.4 6905.6 4.8 6.5 7.8 8.9 1.30 0.0028 HARPS-N 2458121.7229616 39507.2 4.4 6905.8 8.9 6.7 1 8.0 1.317 0.062 HARPS-N 2458121.7229516 39507.2 4.4 6905.8 8.9 6.7 1 8.0 1.317 0.062 HARPS-N 2458121.7229516 39507.2 4.4 6905.8 8.9 6.7 1 8.0 1.317 0.062 HARPS-N 2458141.505522 39506.0 1.2 6915.5 2.3 61.8 5.2 3 1.147 0.010 HARPS-N 2458141.505522 39506.0 1.2 6915.5 2.3 61.8 5.2 3 1.147 0.010 HARPS-N 2458141.505524 39506.0 1.2 6915.5 2.3 61.8 5.2 3 1.140 0.024 HARPS-N 2458141.505524 39506.0 1.2 6915.5 2.3 61.8 5.2 3 1.140 0.024 HARPS-N 2458141.505534 39507.7 2.3 6903.0 4.5 63.2 4.5 1.158 0.029 HARPS-N 2458141.505534 39507.7 2.3 6903.0 4.5 63.2 4.5 1.160 0.024 HARPS-N 2458141.505534 39507.7 2.3 6903.0 4.5 63.2 4.5 1.164 0.017 HARPS-N 2458141.505534 39507.7 2.3 6903.0 4.5 63.2 4.5 1.164 0.017 HARPS-N 2458415.47509444 39507.7 2.3 6903.0 4.5 63.2 4.5 1.164 0.017 HARPS-N 2458415.4550433 3915.7 1.6 6022.3 3.3 79.5 3.3 1.242 0.019 HARPS-N 2458451.5450337 3948.9 1.5 6007.1 3.0 77.3 3.0 1.160 0.015 HARPS-N 2458451.5516377 3948.9 1.5 6007.1 3.0 77.3 3.0 1.180 0.015 HARPS-N 2458451.5516377 3948.9 1.5 6007.1 3.0 77.3 3.0 1.180 0.015 HARPS-N 2458473.56937 3948.9 1.5 6007.1 3.0 77.3 3.0 1.180 0.015 HARPS-N 2458473.56937 3948.9 1.5 6007.1 3.0 77.3 3.0 1.180 0.015 HARPS-N 2458473.56937 3948.9 1.5 6007.1 3.0 60.7 3.4 1.237 0.021 HARPS-N 2458473.56937 3948.9 1.5 6007.1 3.0 60.7 3.4 1.109 0.016 HARPS-N 2458473.56937 3948.9 3.1 6 6007.1 3.0 60.7 3.4 1.109 0.019 HARPS-N 2458473.56937 3948.9 3.1 6 6007.1 3.0 60.7 3.4 1.109 0.019 HARPS-N 3458473.56937 3948.9 1.5 6007.1 3.0 60.7 3.4 1.109 0.019 HARPS-N 3458473.56937 3948.9 1.5 6007.1 3.0 60.7 3.4 1.109 0.019 HARPS-N 3458473.56937 3948.9 3.6 6007.1 3.0 60.7 3.4 1.109 0.019 HARPS-N 3458473.56937 3948.										
2458415,61883639 39607.7 2.4 6965.6 4.8 66.5 4.8 1.130 0.028 HARPS-N 2458161,61883631 39500.0 1.4 6016.4 2.9 68.7 7.8 2.9 1.103 0.015 HARPS-N 2458161,6188361 39500.0 34.4 6037.6 2.8 74.8 2.8 1.240 0.014 HARPS-N 2458142,76620848 39500.0 1.2 6011.5 2.3 68.8 6.7 7.8 1.131 0.008 HARPS-N 245814,7162034 39500.0 1.2 6011.5 2.3 68.8 1.131 0.008 HARPS-N 245814,7162034 39500.1 1.8 6917.5 3.6 75.5 3.6 1.160 0.020 HARPS-N 2458148,7112034 39500.1 1.8 6917.5 3.6 75.5 3.6 1.160 0.020 HARPS-N 2458149,0034044 39511.7 1.6 6925 12 81 12 1.17 0.11 1.7 0.11 HARPS-N 2458149,0034044 39511.7 1.6 6925 12 81 12 1.17 0.11 1.7 0.11 HARPS-N 2458143,0034043 39511.7 1.6 6925.5 3.3 692.2 3.3 1.164 0.017 HARPS-N 2458143,0034034 39511.7 1.6 6923.5 3.3 692.2 3.3 1.164 0.017 HARPS-N 2458143,00303 39493 9.1 6.6 6014.4 3.3 78.0 3.3 1.242 0.019 HARPS-N 2458153,002033 39493 9.1 6.6 6014.4 3.3 78.0 3.3 1.242 0.019 HARPS-N 2458153,002033 39493 9.1 6.6 6014.4 3.3 78.0 3.3 1.122 0.019 HARPS-N 2458153,002033 39493 9.1 6.6 6014.4 3.3 78.0 3.3 1.124 0.019 HARPS-N 2458153,002033 39493 9.1 6.6 6014.4 3.3 78.0 0.3 1.180 0.016 HARPS-N 2458154,1568356 38509.7 1.7 6050.3 3.0 68.5 3.0 1.180 0.016 HARPS-N 2458154,1568356 38509.7 1.7 6050.3 3.0 68.5 3.0 1.180 0.016 HARPS-N 2458164,4560789 3949.6 1.5 6007.1 3.0 7.7 3.3 0.0 1.180 0.016 HARPS-N 2458174,56083109 3949.6 1.1 6011.6 2.2 66.0 2.2 1.1493 0.0099 HARPS-N 2458174,56083109 3949.6 1.1 6011.6 2.2 66.0 2.2 1.1493 0.0099 HARPS-N 2458174,56083109 3949.6 1.1 6011.6 2.2 66.0 2.2 1.1493 0.0099 HARPS-N 2458174,56083109 3949.6 1.1 6011.6 2.2 66.0 2.2 1.1493 0.0099 HARPS-N 2458174,56083109 3949.6 1.1 6011.6 2.2 66.0 2.2 1.1493 0.0099 HARPS-N 2458174,56083109 3949.6 1.1 6011.6 2.2 66.0 2.2 1.1493 0.0099 HARPS-N 2458174,56083109 3949.6 6 1.0 601.2 2.7 7.7 8.8 7.7 1.1 1.2 0.001 HARPS-N 2458174,56083109 3949.6 6 1.1 601.6 0.000 3.3 66.3 3.9 1.140 0.017 HARPS-N 2458174,56083109 3949.6 6 1.1 601.6 0.000 3.3 66.3 3.9 1.140 0.019 HARPS-N 2458174,56083109 3949.6 6 1.0 600.0 3.3 66.0 2.2 1.1493 0.0099 HARPS-N 245818,56031833 3949.6										
2458415,72034413 39604.5 1.4 6916.4 2.9 68.7 2.9 1.163 0.015 HARPS-N 2458412,7229016 39407.8 1.4 6937.6 2.8 74.8 74.8 2.8 1.240 0.014 HARPS-N 2458412,7229016 39407.8 1.0 6025.8 8.0 67.1 8.0 1.317 0.062 HARPS-N 2458415,700343 39506.2 1.2 691.5 1.3 6.3 6.3 1.317 0.062 HARPS-N 2458415,5005249 39506.0 1.2 691.5 1.3 6.3 6.3 8.2 3.1 1.37 0.006 HARPS-N 2458414,5005249 39506.0 1.2 691.5 2.3 6.8 8.0 1.317 0.010 HARPS-N 2458414,5005249 39506.0 1.2 691.5 2.3 6.8 8.2 3.1 1.37 0.010 HARPS-N 2458414,94304120 39518.1 1.8 691.5 2.3 6.8 8.2 3.1 1.37 0.010 HARPS-N 2458414,94304120 39518.1 7.2 3 608.0 4.5 6.3 2.2 4.5 1.150 0.029 HARPS-N 2458414,94304120 39518.1 7.2 3 608.0 4.5 6.3 2.2 4.5 1.150 0.029 HARPS-N 2458414,94304120 39518.1 7.2 3 608.0 4.5 6.3 2.2 4.5 1.150 0.029 HARPS-N 2458414,9605441 39517.7 2.3 608.0 4.5 6.3 2.2 4.5 1.150 0.029 HARPS-N 2458436,4605477 3940.9 1.6 6022.3 3.3 79.5 5.3 1.151 0.017 HARPS-N 2458436,4605787 3940.9 1.6 6022.3 3.3 79.5 5.3 3.0 1.150 0.017 HARPS-N 2458454.0 4.0 1.2 1.2 1.1 1.1 1.1 1.1 1.1 1.1 1.1 1.1	2458410.73761710	39506.9	2.7	6904.2		81.5	5.4	1.143	0.037	HARPS-N
2458421.64508561 39500.0 1.4 6937.6 2.8 74.8 2.8 1.240 0.014 HARPS-N 2458421.65051751 39505.2 4.4 6932.8 8.8 65.0 67.1 8.0 1.317 0.002 HARPS-N 2458424.65081781 39505.2 4.4 6922.8 8.8 65.0 68.8 1.255 0.068 HARPS-N 2458424.65081781 39505.2 4.2 9 6016.1 5.5 60.5 5.7 7.1 1.247 0.014 HARPS-N 245844.65053020 39506.1 1.8 6917.5 3.6 67.5 3.6 1.100 0.020 HARPS-N 245844.650530210 39506.1 1.8 6917.5 3.6 67.5 3.6 1.100 0.020 HARPS-N 2458444.650530210 39518.1 5.9 6025 1.8 1 12 1.17 0.11 HARPS-N 2458444.65053041 39507.7 1.6 6903.5 3.2 60.2 3.2 1.164 0.017 HARPS-N 2458444.65053041 39507.7 1.6 6903.5 3.2 60.2 3.2 1.164 0.017 HARPS-N 2458454.6507387 3949.5 1.6 6923.5 3.3 75.5 3.3 1.165 0.017 HARPS-N 2458454.45057387 3949.5 1.6 6922.3 3.3 75.5 3.3 1.165 0.017 HARPS-N 2458454.45057387 3949.5 1.6 6902.0 3.1 77.7 3.1 1.155 0.017 HARPS-N 2458454.45057387 3949.5 1.5 6902.0 3.1 77.7 3.1 1.155 0.017 HARPS-N 2458454.45057387 3949.5 1.5 6902.0 3.1 77.7 3.1 1.155 0.017 HARPS-N 2458454.45057387 3949.5 1.5 6902.0 3.1 77.7 3.1 1.155 0.017 HARPS-N 2458454.65057387 3949.5 1.5 6902.0 3.1 77.7 3.1 1.155 0.017 HARPS-N 2458454.65057387 3949.5 1.5 6902.0 3.1 77.7 3.1 1.155 0.017 HARPS-N 2458454.65057387 3949.5 1.5 6902.0 3.1 77.7 3.1 1.155 0.017 HARPS-N 2458454.65057387 3949.5 1.3 6901.9 2.5 77.2 2.5 1.009.0 0.01 HARPS-N 2458454.65057387 3949.5 1.3 6901.0 2.5 7.7 1.2 1.2 1.2 1.2 1.2 1.2 1.2 1.2 1.2 1.2	2458415.61383639	39507.7	2.4	6905.6				1.130		HARPS-N
2458421.72295016 39497.8 4.0 9953.8 8.0 67.1 8.0 1.317 0.062 HARPS-N 2458424.7602984 39505.2 4.4 9692.8 8.8 63.0 8.8 1.255 0.062 HARPS-N 2458424.7602984 39505.2 1.2 6911.5 7.3 63.8 2.3 1.137 0.061 HARPS-N 2458424.7602984 39506.0 1.2 6911.5 2.3 63.8 2.3 1.137 0.061 HARPS-N 245844.5695249 39506.0 1.2 6911.5 2.3 63.8 2.3 1.137 0.061 HARPS-N 245844.5695249 39506.0 1.2 6911.5 2.3 63.8 2.3 1.137 0.061 HARPS-N 245844.56963404 39506.1 1.2 6911.5 2.3 63.8 2.3 1.137 0.061 HARPS-N 245844.56963404 39506.7 7 2.3 6913.5 3.2 692.2 4.5 1.158 0.002 HARPS-N 2458445.47509484 39511.7 1.6 6923.5 3.2 692.2 3.2 1.164 0.017 HARPS-N 2458451.47509484 39511.7 1.6 6923.5 3.2 692.2 3.2 1.164 0.017 HARPS-N 2458453.60424787 39495.9 1.6 6922.3 3.3 79.5 3.3 1.242 0.019 HARPS-N 2458453.60424787 39495.9 1.6 6922.3 3.3 79.5 3.3 1.242 0.019 HARPS-N 2458453.60424787 39495.9 1.6 6922.3 3.3 79.5 3.3 1.242 0.019 HARPS-N 2458453.60424787 39495.9 1.6 6912.4 3.3 78.0 3.3 1.173 0.019 HARPS-N 2458453.60424787 39495.9 1.6 6912.4 3.3 78.0 3.3 1.173 0.019 HARPS-N 2458452.60424787 39492.6 1.5 6912.4 3.3 78.0 3.3 1.173 0.019 HARPS-N 2458452.664838556 3950.7 1.7 6915.3 3.4 60.7 3.4 1.237 0.021 HARPS-N 2458452.664838556 3950.7 1.7 6915.3 3.4 60.7 3.4 1.237 0.021 HARPS-N 2458454.6650996 39494.9 1.3 6901.9 2.7 74.8 2.7 1.668 0.012 HARPS-N 2458474.5698190 39492.6 1.3 6901.9 2.7 74.8 2.7 1.668 0.012 HARPS-N 2458474.5698190 39492.6 1.3 6901.3 690.3 1.7 76.0 2.7 1.66 0.0 1.2 1.478-N 2458474.5698190 39492.6 1.3 6901.3 2.6 66.0 2.2 1.1493 0.009 HARPS-N 2458474.5698190 39492.6 1.3 6901.3 2.6 66.0 2.2 1.1493 0.009 HARPS-N 2458475.5043855 3950.5 2.9 6915.2 5.8 70.1 5.8 1.161 0.034 HARPS-N 2458475.504385 3950.5 2.9 6915.2 5.8 70.1 5.8 1.161 0.034 HARPS-N 2458475.504385 3950.5 2.9 6915.2 5.8 70.1 5.8 1.161 0.034 HARPS-N 2458475.504385 3950.5 2.9 6915.2 5.8 70.1 5.8 1.110 0.004 HARPS-N 2458475.504385 3950.5 2.9 6915.2 5.8 70.1 5.8 6.1 1.10 0.004 HARPS-N 2458475.504385 3950.5 2.9 6915.2 5.8 70.1 5.8 6.0 0.0 2.2 1.1493 0.009 HARPS-N 2458475.504385 3950.5 2.1 6090.3 2.4 605.5 74.										
2458424.69841781 93950.2										
2458424.76629848 39502.2 2.9 6916.1 5.7 69.5 5.7 1.247 0.041 IMARPS-N 245844.45120394 39506.1 1.2 6911.5 2.3 68.8 2.3 1.137 0.01 IMARPS-N 245844.45120394 39506.1 1.8 6917.5 3.6 75.5 3.6 1.160 0.020 IMARPS-N 245844.49.69643641 39507.7 2.3 6903.0 4.5 63.2 81 12 1.17 0.11 IMARPS-N 245844.969643641 39507.7 2.3 6903.0 4.5 63.2 4.5 1.158 0.029 IMARPS-N 2458461.4509444 39511.7 1.6 6923.5 3.2 69.2 3.2 1.164 0.01 IMARPS-N 2458461.4509383 3949.5 1.6 6922.3 2.3 692.3 3.2 1.164 0.01 IMARPS-N 2458451.4509383 3949.5 1.6 6922.3 3.2 69.2 3.2 1.124 0.01 IMARPS-N 2458451.4509387 3949.5 1.5 6902.0 3.1 75.7 3.1 1.155 0.017 IMARPS-N 2458451.4509387 3949.5 1.5 6902.0 3.1 75.7 3.1 1.155 0.017 IMARPS-N 2458454.4509387 3949.5 1.5 6902.0 3.1 75.7 3.1 1.155 0.017 IMARPS-N 2458454.4509387 3949.5 1.5 6902.1 3.3 6907.1 3.0 77.3 3.0 1.189 0.016 IMARPS-N 2458454.4509387 3949.5 1.5 6907.1 3.0 673.3 4.0 0.7 3.4 1.1237 0.017 IMARPS-N 2458454.4509387 3949.5 1.5 6907.1 3.0 673.5 3.4 60.7 3.4 1.237 0.01 IMARPS-N 2458454.4509380 3949.9 1.3 6911.9 2.5 73.2 2.5 1.092 0.011 IMARPS-N 2458454.4509380 3949.1 1.3 6911.9 2.5 73.2 2.5 1.092 0.011 IMARPS-N 2458454.4509380 3949.1 1.3 6913.1 2.7 74.8 2.7 1.068 0.012 IMARPS-N 2458454.4509380 3949.1 1.3 6913.1 2.7 75.2 1.1068 0.012 IMARPS-N 2458474.47138988 3949.1 1.3 6913.1 2.7 75.2 1.0 0.0 1.180 0.012 IMARPS-N 2458474.5409380 3949.1 1.3 6913.1 2.2 60.0 0.0 1.2 1.180 0.002 IMARPS-N 2458474.5409380 3949.1 1.3 6913.1 2.2 60.0 0.0 1.2 1.180 0.002 IMARPS-N 2458474.5409380 3949.1 1.3 6913.1 2.2 60.0 0.0 0.0 0.0 0.0 0.0 0.0 0.0 0.0 0.										
2458445.59050249 39590.0 1.2 9911.5 2.3 63.8 2.3 1.137 0.010 HARPS-N 2458444.5905120 39518.1 5.9 6925 12 81 12 1.17 0.11 HARPS-N 2458449.42303120 39518.1 1.6 6923.5 1.2 81 12 1.17 0.11 HARPS-N 2458449.42303120 39518.1 1.6 6923.5 3.2 4.5 1.158 0.029 HARPS-N 2458451.47509484 39511.7 1.6 6923.5 3.2 4.5 1.158 0.029 HARPS-N 2458451.47509484 39511.7 1.6 6923.5 3.2 3.2 1.164 0.017 HARPS-N 2458451.47509484 39511.7 1.6 6923.5 3.2 3.2 1.164 0.017 HARPS-N 2458451.47509484 39511.7 1.6 6923.5 3.2 3.2 1.164 0.017 HARPS-N 2458451.47509484 39511.7 1.6 6923.5 3.2 3.2 1.164 0.017 HARPS-N 2458451.47509487 3949.5 1.6 6914.4 3.3 78.0 3.3 1.173 0.019 HARPS-N 2458451.59126787 3948.9 1.5 6902.0 3.1 75.7 3.1 1.155 0.017 HARPS-N 2458451.59126787 3948.9 1.5 6902.0 3.1 75.7 3.1 1.155 0.017 HARPS-N 2458451.59126377 3948.9 1.5 6902.0 3.0 68.5 3.0 1.180 0.015 HARPS-N 2458451.59126377 3948.9 1.3 6911.9 2.5 73.2 2.5 1.002 0.011 HARPS-N 2458451.5912637 3948.9 1.3 6911.9 2.5 73.2 2.5 1.002 0.011 HARPS-N 2458475.691896 3991.9 1.3 6911.9 2.5 73.2 2.5 74.2 2.5 1.002 0.011 HARPS-N 2458475.691896 3991.9 1.3 6911.9 2.5 73.2 2.5 74.8 2.2 1.168 0.012 HARPS-N 2458475.691809 3991.9 1.3 6911.9 2.5 73.2 2.5 74.8 2.2 1.168 0.012 HARPS-N 2458477.5029455 3950.5 2.9 6915.2 5.8 70.1 5.8 1.164 0.039 HARPS-N 2458477.5029455 3950.5 2.9 6915.2 5.8 70.1 5.8 1.164 0.039 HARPS-N 2458477.5029455 3950.5 2.9 6915.2 5.8 70.1 5.8 1.164 0.039 HARPS-N 2458477.5029455 3950.5 2.9 6915.2 5.8 70.1 5.8 1.164 0.021 HARPS-N 2458477.5029455 3950.5 2.9 6915.2 5.8 70.1 5.8 1.164 0.021 HARPS-N 2458477.5029455 3950.5 2.9 6915.2 5.8 70.1 5.8 1.164 0.021 HARPS-N 2458475.5029587 3999.3 1.1 6911.6 2.2 66.0 2.2 1.143 0.009 HARPS-N 2458475.5029587 3999.3 1.1 6911.8 691.3 2.2 66.9 2.2 1.223 0.010 HARPS-N 2458475.5029587 3999.3 1.1 6911.8 691.3 2.2 66.9 2.8 1.174 0.016 HARPS-N 2458475.5029587 3999.3 1.1 6911.8 691.3 2.2 66.9 2.8 1.174 0.016 HARPS-N 2458475.502587 3999.5 1.1 6911.8 691.3 2.2 66.9 2.2 1.144 0.009 HARPS-N 2458475.502587 3999.5 3.1 1.0 6911.9 1.1 6911.8 1.1 6911.8 1.1 6911.8 1.1 691										
2458448-71120394 39506.1 1.8 6917.5 3.6 75.5 3.6 1.160 0.020 IARPS-N 2458449-69543041 39507.7 2.3 6903.0 4.5 63.2 4.5 1.158 0.029 IARPS-N 2458449-69543041 39507.7 2.3 6903.0 4.5 63.2 4.5 1.158 0.029 IARPS-N 2458419-6954984 39511.7 1.6 6923.5 3.2 69.2 3.2 1.164 0.017 HARPS-N 2458419-6954984 39511.7 1.5 6917.5 2.9 68.5 2.9 1.184 0.015 HARPS-N 2458419-6954787 39495.9 1.5 6902.0 3.1 75.7 3.3 1.224 0.019 HARPS-N 2458451-456507857 39492.6 1.5 6902.0 3.1 75.7 3.3 1.125 0.017 HARPS-N 2458454-64567857 39499.9 1.5 6902.0 3.1 75.7 3.0 1.185 0.015 IARPS-N 2458454-64567857 39499.7 1.5 6895.0 3.0 68.5 3.0 1.189 0.016 HARPS-N 2458454-64568556 39507 1.7 6915.3 3.4 60.7 3.4 1.237 0.021 HARPS-N 2458454-64568556 39507 1.7 6915.3 3.4 60.7 3.4 1.237 0.021 HARPS-N 2458454-64568556 39507 1.7 6915.3 3.4 60.7 3.4 1.237 0.021 HARPS-N 2458475-69487550 39492.6 1.3 6911.9 2.5 73.2 2.5 1.092 0.011 HARPS-N 2458475-69487550 39492.6 1.3 6911.9 2.5 73.2 2.5 1.092 0.011 HARPS-N 2458474-7159808 39494.1 1.3 6913.1 2.7 76.0 2.7 1.007 0.012 HARPS-N 2458474-7159808 39494.1 1.3 6913.1 2.7 76.0 2.7 1.007 0.012 HARPS-N 2458475-6928010 39494.9 1.1 6911.2 2.7 76.0 2.7 1.007 0.012 HARPS-N 2458475-6928010 39494.1 1.3 6913.1 2.7 76.0 2.7 1.007 0.012 HARPS-N 2458475-6928010 39494.1 1.3 6913.1 2.7 76.0 2.7 1.007 0.012 HARPS-N 2458475-6928010 39494.1 1.3 6913.1 2.7 76.0 2.7 1.007 0.012 HARPS-N 2458475-6928010 39494.1 1.3 6913.1 2.7 76.0 2.7 1.007 0.012 HARPS-N 2458475-6928010 39494.1 1.3 6913.1 2.7 76.0 2.7 1.007 0.012 HARPS-N 2458475-6928010 39494.1 1.3 6913.0 2.7 74.5 2.7 1.008 0.012 HARPS-N 2458475-5928010 39494.1 1.3 6913.1 2.7 76.0 2.7 1.007 0.012 HARPS-N 2458475-5928010 39494.1 1.3 6913.1 2.7 76.0 2.7 1.007 0.012 HARPS-N 2458478-59058010 39494.1 1.3 6913.1 2.7 76.0 2.7 1.007 0.012 HARPS-N 2458478-59058010 39494.1 1.3 6913.1 2.7 76.0 2.7 1.007 0.012 HARPS-N 2458478-59058010 39494.1 1.3 6913.1 2.7 76.0 2.7 1.007 0.012 HARPS-N 2458481-59058010 39494.1 1.3 6913.1 2.7 76.0 2.7 1.007 0.012 HARPS-N 2458478-59058010 39494.1 1.3 6913.1 2.7 76.0 2.7 1.1 1.007 0.009										
2458449.42303120 39518.1 5.9 6925 12 81 12 1.17 0.11 IARPS-N 2458449.42303140 39511.7 1.6 6923.5 3.2 69.2 3.2 1.164 0.017 IARPS-N 2458451.47509484 39511.7 1.6 6923.5 3.2 69.2 3.2 1.164 0.017 IARPS-N 2458451.47509484 39511.7 1.6 692.3 3.3 79.5 3.3 1.22 0.019 IARPS-N 2458453.60424787 30495.9 1.6 6922.3 3.3 79.5 3.3 1.273 0.019 IARPS-N 2458453.60424787 30495.9 1.6 6922.3 3.3 79.5 3.3 1.273 0.019 IARPS-N 2458453.60424787 30495.9 1.6 6922.3 3.3 79.5 3.3 1.273 0.019 IARPS-N 2458454.6567987 30495.9 1.6 6922.3 3.0 75.7 3.1 1.11.5 0.017 IARPS-N 2458454.6567987 30492.9 1.5 6902.0 3.0 75.7 3.1 1.11.5 0.017 IARPS-N 245846.46567887 30492.9 1.5 6902.0 3.0 66.5 3.0 0.1 1.08 0.016 IARPS-N 245846.66688556 30509.7 1.7 6915.3 3.4 60.7 3.4 1.237 0.021 IARPS-N 2458462.64688556 30509.7 1.7 6915.3 3.4 60.7 3.4 1.237 0.021 IARPS-N 2458473.63947550 30492.6 1.3 6909.0 2.7 74.8 2.7 1.008 0.016 IARPS-N 2458474.56083109 30491.4 1.3 6911.9 2.5 73.2 2.5 1.002 0.011 IARPS-N 2458474.56083109 30491.4 1.3 6913.4 2.2 76.0 2.7 1.006 0.012 IARPS-N 2458474.56083109 30491.4 1.3 6913.4 2.2 76.0 2.7 1.007 0.012 IARPS-N 2458477.50920857 39503.8 3.4 6950.6 6.7 64.1 6.7 1.120 0.048 IARPS-N 2458477.60820837 39503.8 3.4 6950.6 6.7 64.1 6.7 1.120 0.048 IARPS-N 2458474.56083109 30491.6 1.1 6911.6 2.2 76.0 0.1 5.8 1.104 0.039 IARPS-N 2458474.5608370 30491.6 1.1 6911.6 2.2 76.0 0.1 5.8 1.104 0.039 IARPS-N 2458474.5608370 30491.6 1.1 6911.6 2.2 76.0 0.1 5.8 1.104 0.039 IARPS-N 2458474.5608370 30491.5 1.9 6914.6 3.3 60.9 3.8 1.104 0.02 IARPS-N 2458474.5608370 30491.6 1.1 6914.6 3.8 66.9 3.8 1.164 0.02 IARPS-N 24584875.5045588 3050.0 1.5 6806.6 3.8 60.9 3.8 1.164 0.02 IARPS-N 24584875.5045588 3050.0 1.5 6806.6 3.8 60.9 3.8 1.104 0.02 IARPS-N 2458481.5066002 30494.5 1.9 6806.6 3.8 60.9 3.8 1.104 0.02 IARPS-N 2458481.50366002 30494.5 1.9 6806.6 3.8 60.9 3.8 1.104 0.02 IARPS-N 3458481.50366002 30494.5 1.9 6806.6 3.8 60.9 3.8 1.104 0.02 IARPS-N 3458481.50366002 30494.5 1.9 6806.6 3.8 60.2 3.8 1.104 0.02 IARPS-N 3458481.50366002 30494.5 1.9 6806.6 3.8 60.2 3.3 1.100 0.										
2458449,69543641 39507.7										
2458451.61304290 39512.1 1.5 6917.5 2.9 68.5 2.9 1.184 0.015 HARPS-N 2458454.5424787 34945.9 1.6 6912.4 3.3 78.0 3.3 1.242 0.019 HARPS-N 2458454.5420377 3498.9 1.6 6902.0 3.1 75.7 3.1 1.155 0.017 HARPS-N 2458454.55420377 3498.9 1.5 6907.1 3.0 77.3 3.0 1.180 0.015 HARPS-N 245845.45420377 3498.9 1.5 6907.1 3.0 77.3 3.0 1.180 0.016 HARPS-N 245845.45420377 3498.9 1.5 6907.1 3.0 690.5 3.0 68.5 3.0 1.198 0.016 HARPS-N 245845.64471787 34949.7 1.5 6915.3 3.4 60.7 3.4 1.237 0.021 HARPS-N 245845.64471787 34949.7 1.5 6915.3 3.4 60.7 3.4 1.237 0.021 HARPS-N 245847.54919.0 3494.9 1.3 6911.9 2.7 72.8 2.5 1.692 0.011 HARPS-N 245847.54919.0 3494.9 1.3 6911.9 2.7 72.8 2.5 1.692 0.011 HARPS-N 245847.54919.0 3494.9 1.3 6911.9 2.2 66.0 2.2 1.1493 0.000 99 HARPS-N 245847.5493803 3494.1 1.3 6913.1 2.7 76.0 2.7 1.067 0.012 HARPS-N 245847.5495455 3495.0 3494.1 1.3 6913.1 2.7 76.0 2.7 1.067 0.012 HARPS-N 245847.549545 3495.0 3494.9 1.3 6950.6 6.7 6.4 1.1 6.7 1.120 0.009 HARPS-N 245847.54954568 3950.2 1.3 6950.6 6.7 6.4 1.1 6.7 1.120 0.009 HARPS-N 245847.54954568 3950.2 0.1 3 6917.9 2.7 72.5 2.7 1.250 0.013 HARPS-N 245847.54954568 3950.2 0.1 3 6917.9 2.7 72.5 2.7 1.250 0.013 HARPS-N 245847.54954568 3950.2 0.1 3 6917.9 2.7 72.5 2.7 1.250 0.013 HARPS-N 245847.54954568 3950.2 0.1 3 6917.9 2.7 72.5 2.7 1.250 0.013 HARPS-N 2458479.54013997 3997.3 1.1 6919.3 2.2 66.9 2.2 1.223 0.010 HARPS-N 2458479.54013997 3997.3 1.1 6919.3 2.2 66.9 2.2 1.223 0.010 HARPS-N 2458480.9811363 3494.5 1.6 6904.6 3.3 80.0 3.3 1.164 0.021 HARPS-N 2458480.9811363 3499.5 1.6 6904.6 3.3 80.0 3.3 1.164 0.021 HARPS-N 2458480.9811363 3499.5 1.6 6904.6 3.3 80.0 3.3 1.164 0.021 HARPS-N 2458480.9811363 3499.5 1.6 6904.6 3.3 80.0 3.3 1.164 0.021 HARPS-N 2458480.9811363 3499.5 1.6 6904.6 3.8 77.7 1.250 0.013 HARPS-N 2458480.9811363 3499.5 1.6 6904.6 3.3 80.0 3.3 1.164 0.021 HARPS-N 2458480.9811363 3499.5 1.6 6904.6 3.3 80.0 3.3 1.164 0.021 HARPS-N 3458480.9811363 3499.5 1.6 6904.6 3.3 80.0 3.3 1.164 0.021 HARPS-N 3458480.9811363 3499.5 1.6 6904.6 3.3 80.0 3.3 1.164 0.021 HARPS										
2458453.60424787 3949.9 1.6 692.3 3.3 79.5 3.3 1.242 0.019 HARPS-N 2458454.6507987 3949.2 1.5 6902.0 3.1 75.7 3.1 1.155 0.017 HARPS-N 2458454.6507987 3949.2 1.5 6907.1 3.0 77.3 3.0 1.180 0.015 HARPS-N 245845.6547471787 39499.7 1.5 6895.0 3.0 68.5 3.0 1.198 0.016 HARPS-N 245845.654547471787 39499.7 1.5 6895.0 3.0 68.5 3.0 1.198 0.016 HARPS-N 245845.65458356.03683556 39509.7 1.7 6915.3 3.4 60.7 3.4 1.237 0.021 HARPS-N 2458456.0383556 39509.7 1.7 6915.3 3.4 60.7 3.4 1.237 0.021 HARPS-N 2458475.63947550 3949.9 1.3 6911.9 2.5 73.2 2.5 1.092 0.011 HARPS-N 2458475.63947550 3949.5 1.3 6919.0 2.7 74.8 2.7 1.066 0.012 HARPS-N 2458475.63947550 3949.1 1.3 6913.1 2.2 76.0 2.7 1.067 0.012 HARPS-N 2458475.6394750 3949.1 1.3 6913.1 2.2 76.0 2.7 1.067 0.012 HARPS-N 2458475.6394750 3949.1 1.3 6913.1 2.2 76.0 2.7 1.067 0.012 HARPS-N 2458475.6394750 3949.1 1.3 6915.1 2.2 76.0 2.7 1.067 0.012 HARPS-N 2458475.639473093 3950.7 1.9 6914.6 8.8 60.9 3.8 1.16 0.038 HARPS-N 2458475.504568 3950.2 1.3 6917.9 2.7 72.5 2.7 1.250 0.013 HARPS-N 2458475.504568 3950.2 1.3 6917.9 2.7 72.5 2.7 1.250 0.013 HARPS-N 2458475.504568 3950.2 1.3 6917.9 2.7 72.5 2.7 1.250 0.013 HARPS-N 2458470.59381363 3949.5 1.6 6904.6 3.8 60.9 3.8 1.16 0.004 HARPS-N 24584875.504568 3950.2 1.3 6917.9 2.7 72.5 2.7 1.250 0.013 HARPS-N 24584875.504568 3950.2 1.3 6917.9 2.7 72.5 2.7 1.250 0.013 HARPS-N 2458480.61833460 3950.4 3.3 6922.6 6.5 74.6 6.5 2.4 1.235 0.012 HARPS-N 2458481.61815376 3950.0 1.5 6893.8 2.9 74.9 2.9 1.174 0.016 HARPS-N 2458481.61815376 3950.0 1.5 6893.8 2.9 74.9 2.9 1.174 0.016 HARPS-N 2458481.61815376 3950.0 1.5 6893.8 2.9 74.9 2.9 1.174 0.016 HARPS-N 2458481.5187474767 3950.0 1.5 6893.8 2.9 74.9 2.9 1.174 0.016 HARPS-N 2458481.51874767 3950.5 1.4 6892.5 2.8 66.2 2.8 1.120 0.013 HARPS-N 2458481.518736 3950.0 1.5 6893.8 2.9 74.9 2.9 1.174 0.016 HARPS-N 2458481.51873079 3950.0 1.5 6893.8 2.9 74.9 2.9 1.174 0.016 HARPS-N 3458481.51815376 3950.0 1.5 6893.8 2.9 6896.6 2.6 70.6 2.6 1.118 0.012 HARPS-N 2458481.51873079 3950.0 1.8 6894.0 3.6 66.5 3.8 74.5 1.100	2458451.47509484	39511.7		6923.5	3.2	69.2	3.2	1.164		
2458453.70820393 3949.9.6 1.5 6992.0 3.1 75.7 3.1 1.153 0.019 HARPS-N 2458454.55426377 3948.9.9 1.5 6907.1 3.0 77.3 3.0 1.180 0.015 HARPS-N 2458454.55426377 3948.9.9 1.5 6895.0 3.0 68.5 3.0 1.180 0.015 HARPS-N 2458462.64638556 39509.7 1.7 6915.3 3.4 60.7 3.4 1.237 0.021 HARPS-N 2458462.64638556 39509.7 1.7 6915.3 3.4 60.7 3.4 1.237 0.021 HARPS-N 2458473.63947550 3949.9 1.3 6911.9 2.5 73.2 2.5 1.092 0.011 HARPS-N 2458473.63947550 3949.4 1.3 6901.9 2.5 73.2 2.5 1.092 0.011 HARPS-N 2458473.63947550 3949.4 1 1.3 6913.1 2.7 76.0 2.7 1.067 0.012 HARPS-N 2458474.549398 3949.1 1 1.3 6913.1 2.7 76.0 2.7 1.067 0.012 HARPS-N 2458474.56924955 39505.5 2.9 6915.2 5 8 70.1 5.8 1.164 0.039 HARPS-N 2458474.56924955 39505.5 2.9 6915.2 5.8 70.1 5.8 1.164 0.039 HARPS-N 2458474.59437493 3950.8 3.4 6550.6 6.7 64.1 6.7 1.120 0.048 HARPS-N 2458474.53473093 3950.7 1.9 6914.6 3.8 66.9 3.8 1.64 0.021 HARPS-N 2458475.594568 3950.2 0 1.3 6917.9 2.2 72.5 2.7 1.250 0.013 HARPS-N 2458475.594568 3950.2 0 1.3 6917.9 2.2 72.5 2.7 1.250 0.013 HARPS-N 2458475.594568 39302.0 1.3 6917.9 2.2 72.5 2.7 1.250 0.013 HARPS-N 2458487.5916399 3948.5 1.2 6908.6 3.8 4.6 5.5 2.2 1.235 0.010 HARPS-N 245848.0 1.2505002 39494.5 1.2 6908.6 3.8 74.5 3.8 1.150 0.022 HARPS-N 245848.0 1.2505002 39494.5 1.9 6806.6 3.8 66.9 3.8 1.150 0.02 HARPS-N 245848.1 2.2556002 39494.5 1.9 6806.6 3.8 74.5 3.8 1.150 0.02 HARPS-N 245848.1 2.2556002 39494.5 1.9 6806.6 3.8 74.5 3.8 1.150 0.02 HARPS-N 245848.4 247714376 39502 1.4 6893.7 2.8 66.9 2.8 1.127 0.014 HARPS-N 245848.4 247714376 39502 1.4 6893.7 2.8 66.9 2.8 1.127 0.014 HARPS-N 245848.3 4217046 39506.0 1.5 6808.7 2.9 71.3 2.9 1.177 0.015 HARPS-N 245848.3 4217046 39506.0 1.5 6808.6 3.8 74.5 3.8 1.150 0.02 HARPS-N 245848.3 4217046 39506.0 1.5 6808.5 3.8 66.9 3.8 1.150 0.02 HARPS-N 245848.3 4217046 39506.0 1.5 6808.7 2.5 6806.0 2.8 1.170 0.014 HARPS-N 245848.3 4217049 39506.0 1.5 6808.5 3.1 6609.0 3.9 66.3 3.9 1.206 0.024 HARPS-N 245848.3 4217049 39506.0 1.4 6899.3 3.8 66.0 1.1 0.002 HARPS-N 245848.3 4217049 39506.0 1.7 6809.5 3.3	2458451.61304290									
2458454.46507987 39498.9 1.5 6992.0 3.1 75.7 3.1 1.155 0.017 HARPS-N 2458454.562377 39489.7 1.5 6895.0 3.0 68.5 3.0 1.198 0.016 HARPS-N 2458456.47471787 39499.7 1.5 6895.0 3.0 68.5 3.0 1.198 0.016 HARPS-N 2458452.6463855 39509.7 1.7 6915.3 3.4 60.7 3.4 1.237 0.021 HARPS-N 2458475.54081960 39494.9 1.3 6919.9 2.5 73.2 2.5 1.092 0.011 HARPS-N 2458475.54987550 3949.9 1.3 6919.9 2.7 74.8 2.7 1.068 0.012 HARPS-N 2458474.7133908 39494.1 1.3 6913.1 2.7 75.0 2.7 1.067 0.012 HARPS-N 2458474.739808 39494.1 1.3 6913.1 2.7 75.0 2.7 1.067 0.012 HARPS-N 2458474.7508309 3949.6 1.1 6911.6 2.8 60.0 2.2 1.1439 0.0099 HARPS-N 2458475.508309 3949.6 1.3 6915.0 3.8 70.1 5.8 11.64 0.039 HARPS-N 2458475.508309 3949.3 3.4 6850.6 8 8 6.9 8 8 1.164 0.039 HARPS-N 2458475.508303 3949.3 3.4 6850.6 8 8 6.9 8 8 1.164 0.039 HARPS-N 2458475.508303 3949.3 1.2 6908.3 2.4 66.5 2.2 1.250 0.013 HARPS-N 2458475.508309 3949.3 1.2 6908.3 2.4 66.5 2.4 1.235 0.012 HARPS-N 2458475.508309 3949.5 1.6 6904.6 3.8 6.9 8 8 1.104 0.004 HARPS-N 24584875.504568 3950.5 0.6 9 8 3 2.4 66.5 2.4 1.235 0.012 HARPS-N 24584875.5056002 3949.5 1.6 6904.6 3.3 80.0 3.3 1.164 0.004 HARPS-N 24584815.81933 3949.5 1.6 6904.6 3.8 74.5 4.5 4.5 4.5 4.5 4.5 4.5 4.5 4.5 4.5										
2458454.5646.64638556 39509.7 1.7 6915.3 3.4 60.7 3.4 1.237 0.021 HARPS-N 2458462.64638556 39509.7 1.7 6915.3 3.4 60.7 3.4 1.237 0.021 HARPS-N 2458473.6091890 39194.9 1.3 6911.9 2.5 73.2 2.5 1.092 0.011 HARPS-N 2458473.63947550 39192.6 1.3 6919.0 2.7 74.8 2.7 1.068 0.012 HARPS-N 2458473.63947550 39192.6 1.3 6919.0 2.7 74.8 2.7 1.068 0.012 HARPS-N 2458474.56083109 39194.1 1.3 6919.1 2.7 76.0 2.7 1.067 0.012 HARPS-N 2458474.56083109 39194.1 1.3 6913.1 2.7 76.0 2.7 1.067 0.012 HARPS-N 2458474.56083109 39194.1 1.3 6913.1 2.7 76.0 2.7 1.067 0.012 HARPS-N 2458474.56083109 39194.6 1.1 6911.6 2.2 66.0 2.2 1.1493 0.0099 HARPS-N 2458474.56083109 39194.7 1.9 6915.2 5.8 70.1 5.8 1.164 0.039 HARPS-N 2458477.60820837 39503.8 3.4 6950.6 6.7 64.1 6.7 1.120 0.048 HARPS-N 2458475.5015397 3991.7 1.9 6914.6 3.8 66.9 3.8 1.64 0.021 HARPS-N 2458475.5015397 3917.3 1.1 6919.3 2.2 65.9 2.2 1.230 0.013 HARPS-N 2458475.5015397 3917.3 1.1 6919.3 2.2 65.9 2.2 1.235 0.010 HARPS-N 2458475.5015397 3917.3 1.1 6919.3 2.2 65.9 2.2 1.235 0.010 HARPS-N 2458487.50183163 3918.5 1.6 6904.6 3.3 4.0 6.3 3.0 1.0 4.0 4.0 4.0 4.0 4.0 4.0 4.0 4.0 4.0 4										
2458456.47471787 39499.7 1.5 6895.0 3.0 68.5 3.0 1.198 0.016 HARPS-N 2458473.54081960 39494.9 1.3 6911.9 2.5 73.2 2.5 1.092 0.011 HARPS-N 2458473.54081960 39494.9 1.3 6901.9 2.5 73.2 2.5 1.092 0.011 HARPS-N 2458474.47139808 39494.1 1.3 6913.1 2.7 76.0 2.7 1.067 0.012 HARPS-N 2458474.47139808 39494.1 1.3 6913.1 2.7 76.0 2.7 1.067 0.012 HARPS-N 2458474.5083109 3949.6 1.1 6911.6 2.2 66.0 2.2 1.1493 0.0099 HARPS-N 2458474.50820837 3950.8 2.9 6915.2 5.8 70.1 5.8 1.164 0.039 HARPS-N 2458475.60920837 3950.8 3.4 6950.6 6.7 64.1 6.7 1.120 0.048 HARPS-N 2458478.43374093 39504.7 1.9 6914.6 3.8 66.9 3.8 1.164 0.021 HARPS-N 2458479.54013997 39497.3 1.1 6919.3 2.2 65.9 2.2 1.223 0.010 HARPS-N 2458479.54013997 39497.3 1.1 6919.3 2.2 65.9 2.2 1.223 0.010 HARPS-N 2458480.49811363 39498.3 1.2 6908.3 2.4 69.5 2.4 1.235 0.012 HARPS-N 2458480.49811363 39498.5 1.6 6904.6 3.3 80.0 3.3 1.164 0.017 HARPS-N 2458480.49811363 39498.5 1.6 6904.6 3.3 80.0 3.3 1.164 0.017 HARPS-N 2458481.52056002 39494.5 1.9 6896.6 3.8 74.5 3.8 1.150 0.022 HARPS-N 2458481.52056002 39494.5 1.9 6896.6 3.8 74.5 3.8 1.150 0.022 HARPS-N 2458481.52056002 39494.5 1.9 6896.6 3.8 74.5 3.8 1.150 0.022 HARPS-N 2458481.52056002 39494.5 1.9 6896.6 3.8 74.5 3.8 1.150 0.02 HARPS-N 2458481.52056002 39494.5 1.9 6896.6 3.8 74.5 3.8 1.150 0.02 HARPS-N 2458481.52056002 39494.5 1.9 6896.6 5.7 74.6 6.9 2.8 1.127 0.016 HARPS-N 2458481.52056002 39495.5 1.9 6896.6 3.8 74.5 3.8 1.150 0.02 HARPS-N 2458481.52056002 39494.5 1.9 6896.6 3.8 74.5 3.8 1.150 0.02 HARPS-N 2458481.52056002 39495.5 1.9 6896.6 3.8 74.5 3.8 1.150 0.02 HARPS-N 2458481.52056002 39495.5 1.9 6896.6 3.8 74.5 3.8 1.150 0.02 HARPS-N 2458481.52056002 3950.5 1.4 6895.7 2.8 66.9 2.8 1.127 0.016 HARPS-N 2458481.52056002 3950.5 1.4 6895.7 2.8 66.9 2.8 1.127 0.016 HARPS-N 2458481.52056002 3950.5 1.4 6895.7 3.6 66.5 74.6 6.9 2.8 1.120 0.001 HARPS-N 2458582.34130 3950.6 1.4 6895.7 3.6 6895.7 3.8 66.2 2.8 1.120 0.010 HARPS-N 2458581.341443 3800.6 1.4 6899.5 3.8 6894.0 3.6 61.6 6.0 3.6 1.100 0.002 HARPS-N 2458581.34143 3800.6 1.1										
2458473.63947550 39494.9 13. 6911.9 2.5 73.2 2.5 1.092 0.011 HARPS-N 2458473.63947550 39494.9 13. 6911.9 2.5 73.2 2.5 1.092 0.011 HARPS-N 2458473.63947550 39494.9 13. 6911.6 2.2 66.0 2.7 1.067 0.012 HARPS-N 2458474.56983109 39494.1 13. 6913.1 2.7 76.0 2.7 1.067 0.012 HARPS-N 2458474.56983109 39494.1 13. 6913.1 2.7 76.0 2.7 1.067 0.012 HARPS-N 2458474.56983109 39494.1 13. 6913.1 2.7 76.0 2.2 1.1493 0.0099 HARPS-N 2458474.56983109 39494.1 13. 6911.6 2.2 66.0 2.2 1.1493 0.0099 HARPS-N 2458474.56982837 39503.8 3.4 6950.6 6.7 64.1 6.7 1.120 0.048 HARPS-N 2458474.5691337039 39504.7 1.9 6914.6 3.8 66.9 3.8 1.164 0.021 HARPS-N 2458478.55045588 39502.0 1.3 6917.9 2.7 72.5 2.7 1.250 0.013 HARPS-N 2458479.59583870 39498.3 1.2 6908.3 2.4 69.5 2.4 1.235 0.010 HARPS-N 2458479.59583870 39498.3 1.2 6908.3 2.4 69.5 2.4 1.235 0.012 HARPS-N 2458481.61833460 39500.4 3.3 6922.6 6.5 74.6 6.5 1.182 0.0049 HARPS-N 2458481.61813376 39500.0 1.5 6893.8 2.9 74.9 2.9 1.174 0.014 HARPS-N 2458481.61815376 39500.0 1.5 6893.8 2.9 74.9 2.9 1.174 0.016 HARPS-N 2458482.57623761 39502.2 1.4 6893.7 2.8 66.2 2.8 1.127 0.014 HARPS-N 2458482.57623761 39502.2 1.2 6898.0 2.4 67.9 2.4 1.135 0.002 HARPS-N 2458483.61793697 3950.5 1.1 6892.7 2.8 66.2 2.8 1.120 0.013 HARPS-N 2458483.61793697 3950.5 1.4 6893.7 2.8 66.2 2.8 1.120 0.013 HARPS-N 2458484.5621664 39507.2 1.5 6892.7 2.9 71.3 2.9 1.174 0.014 HARPS-N 2458484.5621664 39507.2 1.5 6892.7 2.9 71.3 2.9 1.174 0.014 HARPS-N 2458484.5621664 39507.2 1.5 6893.7 2.8 66.2 2.8 1.120 0.013 HARPS-N 2458484.5621664 39507.3 1.6 6894.0 3.6 66.2 6.7 0.6 2.6 1.118 0.012 HARPS-N 2458484.5621664 39507.3 1.6 6894.0 3.6 66.2 6.7 0.6 2.6 1.118 0.012 HARPS-N 2458484.563502 39505.0 1.4 6899.3 2.8 69.1 2.8 1.192 0.013 HARPS-N 2458484.563502 39505.0 1.4 6899.3 2.8 69.1 2.8 1.192 0.013 HARPS-N 2458484.563502 39505.0 1.4 6899.3 2.8 69.1 2.8 1.192 0.014 HARPS-N 2458484.563503 3950.9 2.6 69.0 5.7 4.1 75.7 4.1 1.221 0.027 HARPS-N 2458484.563503 3950.9 3.8 6.9 6.9 6.9 6.0 3.3 3.9 6.0 0.0 4 HARPS-N 2458484.563503 3950.9 3.5 2.6 690.5 3										
2458473.54081960 39494.9 1.3 6909.0 2.7 74.8 2.5 1.092 0.011 HARPS-N 2458474.47139808 39494.1 1.3 6909.0 2.7 74.8 2.7 1.066 0.012 HARPS-N 2458474.47139808 39494.1 1.3 6913.1 2.7 76.0 2.7 1.067 0.012 HARPS-N 2458474.56083109 39491.6 1.1 6911.6 2.2 66.0 2.2 1.1493 0.0099 HARPS-N 2458474.50820837 39506.5 2.9 6915.2 5.8 70.1 5.8 1.164 0.039 HARPS-N 2458474.3374093 39504.7 1.9 6914.6 3.8 66.9 3.8 1.164 0.021 HARPS-N 2458474.34374093 39504.7 1.9 6914.6 3.8 66.9 3.8 1.164 0.021 HARPS-N 2458474.545478.5645568 39502.0 1.3 6917.9 2.7 72.5 2.7 1.250 0.013 HARPS-N 2458474.545478.5958870 3949.3 1.1 6919.3 2.2 65.9 2.2 1.223 0.010 HARPS-N 2458479.54013997 39497.3 1.1 6919.3 2.2 65.9 2.2 1.223 0.010 HARPS-N 2458480.49811363 39498.3 1.2 6908.3 2.4 69.5 2.4 1.235 0.012 HARPS-N 2458480.49811363 39498.5 1.6 6904.6 3.3 80.0 3.3 1.164 0.017 HARPS-N 2458480.49811363 39498.5 1.6 6904.6 3.8 74.5 3.8 1.150 0.017 HARPS-N 2458481.52056002 39494.5 1.9 6896.6 3.8 74.5 3.8 1.150 0.002 HARPS-N 2458481.52056002 39494.5 1.9 6896.6 3.8 74.5 3.8 1.150 0.002 HARPS-N 2458482.47714376 30502.2 1.4 6893.7 2.8 68.9 2.8 1.157 0.002 HARPS-N 2458482.47714376 30502.2 1.4 6893.7 2.8 68.9 2.8 1.127 0.014 HARPS-N 2458482.47714376 30502.2 1.4 6893.7 2.8 68.9 2.8 1.127 0.014 HARPS-N 2458482.47714376 30502.2 1.4 6893.7 2.8 68.9 2.8 1.127 0.014 HARPS-N 2458483.48217046 30506.5 1.4 6892.5 2.8 66.2 2.8 1.120 0.001 HARPS-N 2458484.45730679 30506.9 1.8 6894.0 3.6 61.6 3.6 1.160 0.002 HARPS-N 2458484.45730679 30506.9 1.8 6894.0 3.6 61.6 3.6 1.160 0.002 HARPS-N 2458484.45730679 30506.9 1.8 6894.0 3.6 61.6 3.6 1.160 0.002 HARPS-N 2458484.45730679 30506.9 1.8 6893.3 2.9 71.3 2.9 1.127 0.015 HARPS-N 2458484.45730679 30506.9 1.8 6894.0 3.6 61.6 3.6 1.160 0.002 HARPS-N 2458484.45730679 30506.9 1.8 6893.3 2.5 66.8 2.5 1.138 0.011 HARPS-N 2458484.45730679 30506.9 1.8 6893.3 3.6 60.0 2.2 7.1 5.7 7.4 1.1 1.2 1.0 0.001 HARPS-N 2458484.45330138 39492.8 1.0 6900.0 3.9 66.3 3.3 7.6 6.2 3.3 1.100 0.001 HARPS-N 2458484.536013038999 3050.9 2.4 601.0 2.5 66.8 3.3 5.0 0.0 0.0 0.0 0.0 0										
2458473.639473503         39494.1         1.3         6690.0         2.7         74.8         2.7         1.068         0.012         HARPS-N           2458474.5083109         39491.6         1.1         6911.6         2.2         66.0         2.2         1.14         0.0099         HARPS-N           2458477.60820837         39506.5         2.9         6915.2         5.8         70.1         5.8         1.120         0.048         HARPS-N           2458478.5504568         39504.7         1.9         6914.6         3.8         66.9         3.8         1.120         0.048         HARPS-N           2458478.5504568         39502.0         1.3         6917.9         2.7         7.2.5         2.7         1.250         0.013         HARPS-N           2458478.9504378         39498.3         1.2         6908.3         2.4         69.5         2.4         1.235         0.012         HARPS-N           2458480.61833460         3950.4         3.3         6922.6         6.5         74.6         6.5         1.182         0.049         HARPS-N           2458481.261633460         3950.0         1.5         6893.8         2.9         74.9         2.9         1.174         0.016         HARPS-										
2458474.47139808 39494.1 1.3 6913.1 2.7 76.0 2.7 1.067 0.012 HARPS-N 2458474.5083109 39491.6 1.1 6911.6 2.2 66.0 2.2 1.1493 0.0099 HARPS-N 2458477.50294855 39506.5 2.9 6915.2 5.8 70.1 5.8 1.164 0.039 HARPS-N 2458478.43374093 3950.3 3.4 6950.6 6.7 64.1 6.7 1.120 0.048 HARPS-N 2458478.43374093 3950.1 1.9 6914.6 3.8 66.9 3.8 1.164 0.021 HARPS-N 2458478.54054568 3950.2 1.3 6917.9 2.7 72.5 2.7 1.250 0.013 HARPS-N 2458479.54013997 39497.3 1.1 6919.3 2.2 65.9 2.2 1.223 0.010 HARPS-N 24584879.54013997 39498.3 1.2 6908.3 2.4 69.5 2.4 1.235 0.012 HARPS-N 2458480.4981363 39498.5 1.6 6904.6 3.3 80.0 3.3 1.164 0.017 HARPS-N 2458480.4981363 39498.5 1.6 6904.6 3.3 80.0 3.3 1.164 0.017 HARPS-N 2458481.52056002 39494.5 1.9 6896.6 3.8 74.5 3.8 1.150 0.022 HARPS-N 2458481.52056002 39494.5 1.9 6896.6 3.8 74.5 3.8 1.150 0.022 HARPS-N 2458482.47714376 3950.2 1.4 6893.7 2.8 68.9 2.8 1.127 0.014 HARPS-N 2458483.48217046 3950.2 1.4 6893.7 2.8 68.9 2.8 1.127 0.014 HARPS-N 2458483.48217046 3950.2 1.4 6893.7 2.8 68.9 2.8 1.127 0.014 HARPS-N 2458483.48217046 3950.2 1.4 6892.5 2.8 66.2 2.8 1.120 0.013 HARPS-N 2458484.4739579 3950.9 1.8 6894.0 3.6 61.6 3.6 1.160 0.020 HARPS-N 2458484.4739579 3950.9 1.8 6894.0 3.6 61.6 3.6 1.160 0.020 HARPS-N 2458484.5221664 3950.7 1.3 6886.6 2.6 70.6 2.8 1.120 0.013 HARPS-N 2458484.5221664 3950.7 1.3 6886.6 2.6 70.6 2.8 1.120 0.013 HARPS-N 2458484.5221664 3950.7 1.3 6886.6 2.6 70.6 2.8 1.120 0.013 HARPS-N 2458484.5221664 3950.7 1.3 6886.6 2.6 70.6 2.8 1.120 0.013 HARPS-N 2458484.5221664 3950.7 1.3 6886.6 2.6 70.6 2.8 1.120 0.013 HARPS-N 2458484.5221664 3950.7 1.3 6886.6 2.6 70.6 2.8 1.120 0.013 HARPS-N 2458484.52363713 3949.6 1.9 6900.0 3.9 66.3 3.9 1.13 0.001 HARPS-N 2458485.23831394 3.9 1.0 6.002 HARPS-N 2458485.23831394 3.9 1.2 6900.0 3.9 66.3 3.9 1.10 0.002 HARPS-N 2458485.23831394 3.9 3.0 6.000 3.9 66.3 3.9 1.206 0.024 HARPS-N 2458486.5361350 3950.5 1.7 6900.0 3.9 66.3 3.9 1.10 0.001 HARPS-N 2458480.336193 3950.5 1.7 6900.0 3.9 66.3 3.9 1.10 0.001 HARPS-N 458850.336193 3950.9 3.1 6.0 6900.0 3.9 66.3 3.9										
2458474.56083109 39491.6 1.1 6911.6 2.2 66.0 2.2 1.1493 0.0099 HARPS-N 2458474.760820837 39506.5 2.9 6915.2 5.8 70.1 5.8 1.164 0.039 HARPS-N 2458478.56045568 39504.7 1.9 6914.6 3.8 66.9 3.8 1.120 0.048 HARPS-N 2458478.55045568 39504.7 1.9 6914.6 3.8 66.9 3.8 1.120 0.013 HARPS-N 2458478.55045568 39502.0 1.3 6917.9 2.7 72.5 2.7 1.250 0.013 HARPS-N 2458479.59583870 39495.3 1.2 6908.3 2.4 69.5 2.4 1.235 0.012 HARPS-N 2458480.61833460 3950.4 3.3 6092.6 6.5 74.6 6.5 1.182 0.049 HARPS-N 2458480.61833460 3950.4 3.3 6092.6 6.5 74.6 6.5 1.182 0.049 HARPS-N 2458484.61833460 3950.4 1.9 6896.6 3.8 74.5 3.8 1.150 0.022 HARPS-N 2458484.8257623761 39502.2 1.4 6893.7 2.8 6893.8 2.9 74.9 2.9 1.174 0.016 HARPS-N 2458482.47714376 39502.2 1.2 6888.0 2.8 67.9 2.8 1.127 0.014 HARPS-N 2458483.48217046 39506.5 1.4 6892.5 2.8 66.2 2.8 1.120 0.013 HARPS-N 2458484.45739679 39506.5 1.4 6892.5 2.8 66.2 2.8 1.120 0.014 HARPS-N 2458484.52621664 39507.8 1.3 6886.6 2.6 70.6 2.6 1.118 0.012 HARPS-N 2458484.52621664 39507.8 1.3 6886.6 2.6 70.6 2.6 1.118 0.012 HARPS-N 2458484.52621664 39507.8 1.3 6886.6 2.6 70.6 2.6 1.130 0.013 HARPS-N 2458484.52621664 39507.2 1.5 6892.7 2.9 71.3 2.9 1.174 0.016 HARPS-N 2458484.52621664 39507.2 1.5 6892.7 2.9 71.3 2.9 1.174 0.016 HARPS-N 2458484.54739679 39506.9 1.8 6894.0 3.6 61.6 3.6 1.160 0.020 HARPS-N 2458484.8454383 3950.8 1.8 6894.0 3.6 61.6 3.6 1.160 0.020 HARPS-N 2458484.8454383 3950.8 1.8 6899.7 3.6 66.2 2.8 1.120 0.013 HARPS-N 2458484.854451383 3950.6 1.4 6899.3 2.8 691.0 2.0 2.8 691.										HARPS-N
2458477.50294855         39506.5         2.9         6915.2         5.8         70.1         5.8         1.164         0.039         HARPS-N           2458478.43374093         39504.7         1.9         6914.6         3.8         66.9         3.8         1.164         0.021         HARPS-N           2458478.5504568         35050.2         1.3         6917.9         2.7         72.5         2.7         1.250         0.013         HARPS-N           2458478.5504568         35050.2         1.3         6917.9         2.7         72.5         2.2         1.23         0.010         HARPS-N           2458479.54013997         39498.3         1.2         6908.3         2.2         65.9         2.2         1.235         0.012         HARPS-N           2458481.6181363         39500.4         3.3         6922.6         6.5         74.6         6.5         1.182         0.049         HARPS-N           2458481.61815376         39500.0         1.5         6893.8         2.9         74.9         2.9         1.174         0.016         HARPS-N           2458482.57623761         39502.2         1.2         68810.2         2.4         67.9         2.4         1.135         0.011         HARPS-										
2454878.43374093         39504.7         1.9         6914.6         3.8         66.9         3.8         1.164         0.021         HARPS-N         2458478.5504568         30502.0         1.3         6917.9         2.7         72.5         2.7         1.250         0.013         HARPS-N         2458479.54013997         39498.3         1.1         6919.3         2.2         65.9         2.2         1.235         0.012         HARPS-N         245848.0         245848.0         333         1.164         0.017         HARPS-N         245848.0         245848.0         3949.5         1.6         6904.6         3.3         80.0         3.3         1.164         0.017         HARPS-N         2458481.618.0         3950.4         3.3         692.6         6.5         74.6         6.5         1.182         0.049         HARPS-N         2458481.618.0         3994.5         1.9         6806.6         3.8         74.5         3.8         1.150         0.022         HARPS-N         2458481.618.618.7         39500.0         1.5         6893.7         2.8         68.9         2.8         1.177         0.014         HARPS-N         2458484.527.7         3950.2         1.4         6893.7         2.8         66.9         2.8         1.2         1.118				6915.2						
2454878.55045568         39502.0         1.3         6917.9         2.7         72.5         2.7         1.250         0.010         HARPS-N           2454879.55583870         39498.3         1.2         6908.3         2.4         69.5         2.4         1.235         0.012         HARPS-N           2458480.49811363         39498.5         1.6         6904.6         3.3         80.0         3.3         1.164         0.017         HARPS-N           2458480.4981363         3950.0         1.3         6922.6         6.5         74.6         6.5         1.162         0.049         HARPS-N           2458480.4981363         3950.0         1.5         6893.8         2.9         74.9         2.9         1.174         0.016         HARPS-N           2458481.52056002         3949.4         6.689.1         2.8         68.9         2.8         1.127         0.014         HARPS-N           2458482.4771467         3950.2         1.4         6893.8         2.4         67.9         2.4         1.135         0.011         HARPS-N           2458483.57932245         3950.7         1.3         6896.6         2.6         70.6         2.6         1.18         0.012         HARPS-N	2458477.60820837	39503.8	3.4	6950.6	6.7	64.1	6.7	1.120	0.048	HARPS-N
2458479.54013997         39497.3         1.1         6919.3         2.2         65.9         2.2         1.223         0.010         HARPS-N           2458480.49811363         39498.5         1.6         6904.6         3.3         80.0         3.3         1.164         0.017         HARPS-N           2458484.61833460         39500.4         3.3         602.6         5         74.6         6.5         1.182         0.049         HARPS-N           245848.152056002         3949.5         1.9         6896.6         3.8         74.5         3.8         1.150         0.022         HARPS-N           245848.1527676         39500.0         1.5         6893.7         2.8         68.9         2.8         1.127         0.014         HARPS-N           245848.4527066         3950.2         1.2         6888.0         2.4         67.9         2.4         1.135         0.011         HARPS-N           245848.4527604         39505.8         1.3         6886.6         2.6         70.6         2.6         1.118         0.012         HARPS-N           245848.458276623761         39507.8         1.3         6886.6         2.6         70.6         2.6         1.118         0.012         HARPS-N <td>2458478.43374093</td> <td>39504.7</td> <td>1.9</td> <td>6914.6</td> <td></td> <td>66.9</td> <td>3.8</td> <td>1.164</td> <td>0.021</td> <td>HARPS-N</td>	2458478.43374093	39504.7	1.9	6914.6		66.9	3.8	1.164	0.021	HARPS-N
2458479.59583870         39498.5         1.6         6904.6         3.3         80.0         3.3         1.164         0.017         HARPS-N           2458480.61833460         39500.4         3.3         6922.6         6.5         74.6         6.5         1.182         0.049         HARPS-N           2458481.520566002         39494.5         1.9         6896.6         3.8         74.5         3.8         1.150         0.022         HARPS-N           2458481.61815376         39500.0         1.5         6893.8         2.9         74.9         2.9         1.174         0.016         HARPS-N           2458482.47714376         39502.2         1.4         6893.7         2.8         68.9         2.8         1.127         0.014         HARPS-N           2458482.57632761         39505.5         1.4         6892.5         2.8         66.2         2.8         1.120         0.013         HARPS-N           2458484.5793679         39506.9         1.8         6894.0         3.6         61.6         3.6         1.160         0.020         HARPS-N           2458487.56221664         39505.2         1.5         6892.7         2.9         71.3         2.9         1.12         2.0         1.4 <td></td>										
2458480.49811363         39498.5         1.6         6904.6         3.3         80.0         3.3         1.164         0.017         HARPS-N           2458480.1813360         3950.4         1.9         6896.6         3.8         74.5         3.8         1.150         0.022         HARPS-N           2458481.6181576         3950.0         1.5         6893.8         2.9         74.9         2.9         1.174         0.016         HARPS-N           2458482.47714376         3950.2         1.2         6888.0         2.4         67.9         2.4         1.137         0.011         HARPS-N           2458483.48217046         3950.2         1.2         6888.0         2.4         67.9         2.4         1.135         0.011         HARPS-N           2458484.5427046         39507.8         1.3         6886.6         2.6         70.6         2.6         1.18         0.012         HARPS-N           2458484.56221664         39507.2         1.5         6892.7         2.9         71.3         2.9         1.12         0.015         HARPS-N           2458487.542630         3950.7         2.9         71.3         2.9         1.12         0.027         HARPS-N           2458487.5487.5454										
2458848.6.1833460         3950.4         3.3         6922.6         6.5         74.6         6.5         1.182         0.049         HARPS-N           245848.1.52056002         39494.5         1.9         6896.6         3.8         74.5         3.8         1.150         0.022         HARPS-N           245848.1.61815376         3950.2         1.4         6893.7         2.8         68.9         2.8         1.127         0.014         HARPS-N           245848.4.57267623761         3950.2.2         1.2         688.0         2.4         6.7.9         2.4         1.135         0.011         HARPS-N           245848.4.57397392245         3950.6.5         1.4         6892.5         2.8         66.2         2.8         1.120         0.013         HARPS-N           245848.4.5739679         3950.6.9         1.8         6894.0         3.6         61.6         3.6         1.160         0.020         HARPS-N           2458484.5621644         3950.5         2.0         6905.7         4.1         75.7         4.1         1.221         0.027         HARPS-N           2458487.4451438         3950.6         1.4         6899.3         2.8         69.1         2.8         1.170         0.015										
2458481.52056002         39494.5         1.9         6896.6         3.8         74.5         3.8         1.150         0.022         HARPS-N           2458481.61815376         39500.2         1.4         6893.7         2.8         68.9         2.8         1.127         0.014         HARPS-N           2458482.57623761         39502.2         1.2         688.0         2.4         67.9         2.4         1.135         0.011         HARPS-N           2458483.57932245         39507.8         1.3         6886.6         2.6         70.6         2.6         1.18         0.012         HARPS-N           2458484.5733679         39507.8         1.3         6886.6         2.6         70.6         2.6         1.18         0.012         HARPS-N           2458484.5733679         39507.2         1.5         6892.7         2.9         71.3         2.9         1.12         0.015         HARPS-N           2458485.6621664         39507.2         1.5         6892.7         2.9         71.3         2.9         1.12         0.015         HARPS-N           2458487.54847         39507.6         1.4         6899.3         2.8         69.1         2.8         1.19         0.015         HARPS-N										HARPS-N
2458481_61815376         39500.0         1.5         6893.8         2.9         74.9         2.9         1.174         0.016         HARPS-N           2458482_47714376         39502_2         1.2         6888.0         2.4         67.9         2.4         1.135         0.011         HARPS-N           2458483_48217046         39506.5         1.4         6892.5         2.8         66.2         2.8         1.120         0.013         HARPS-N           2458484_5739679         39506.9         1.8         6894.0         3.6         61.6         3.6         1.160         0.020         HARPS-N           2458484_5739679         39506.5         1.5         6892.7         2.9         71.3         2.9         1.127         0.015         HARPS-N           245848_56221664         39505.3         2.0         6905.7         4.1         75.7         4.1         1.221         0.027         HARPS-N           2458487.4451438         39506.6         1.4         6899.3         2.8         69.1         2.8         1.192         0.015         HARPS-N           2458487.4451438         39507.1         1.4         6901.2         2.8         69.6         2.8         1.170         0.015         HARPS-N<										
2458482_47714376         39502_2         1.4         6893.7         2.8         68.9         2.8         1.127         0.014         HARPS-N           2458482_57623761         39502_2         1.2         6888.0         2.4         67.9         2.4         1.135         0.011         HARPS-N           2458483_57932245         39507.8         1.3         6886.6         2.6         70.6         2.6         1.118         0.012         HARPS-N           245848_45739679         39506.9         1.8         6894.0         3.6         61.6         2.6         1.118         0.012         HARPS-N           245848_45739679         39506.3         2.0         6905.7         2.9         71.3         2.9         1.127         0.015         HARPS-N           245848_565813502         39505.3         2.0         6905.7         4.1         75.7         4.1         1.221         0.027         HARPS-N           245848_4856184800         39501.7         1.4         6901.2         2.8         69.6         2.8         1.170         0.015         HARPS-N           2458488_48184010         39497.3         1.2         6901.9         2.5         66.8         2.5         1.138         0.012         HARP										
2458482.57623761 39502.2 1.2 6888.0 2.4 67.9 2.4 1.135 0.011 HARPS-N 2458483.48217046 39506.5 1.4 6892.5 2.8 67.06 2.8 1.120 0.013 HARPS-N 2458483.48217046 39507.8 1.3 6886.6 2.6 70.6 2.6 1.118 0.012 HARPS-N 2458484.45739679 39506.9 1.8 6894.0 3.6 61.6 3.6 1.160 0.020 HARPS-N 2458484.45739679 39506.9 1.8 6894.0 3.6 61.6 3.6 1.160 0.020 HARPS-N 2458486.5621664 39507.2 1.5 6892.7 2.9 71.3 2.9 1.127 0.015 HARPS-N 2458486.56213603 39505.3 2.0 6905.7 4.1 75.7 4.1 1.221 0.027 HARPS-N 2458487.44451438 39500.6 1.4 6899.3 2.8 69.1 2.8 1.192 0.015 HARPS-N 2458487.5454500 39501.7 1.4 6901.2 2.8 69.6 2.8 1.170 0.015 HARPS-N 2458488.52873713 39499.6 1.9 6901.9 2.5 66.8 2.5 1.138 0.012 HARPS-N 2458489.58273713 39499.6 1.9 6900.0 3.9 66.3 3.9 1.206 0.024 HARPS-N 2458489.43534717 39496.3 1.8 6899.7 3.6 70.6 3.6 1.193 0.021 HARPS-N 24585489.58136198 39492.8 1.6 6908.5 3.1 67.7 3.1 1.166 0.018 HARPS-N 2458502.53993777 39505.4 2.5 6896.3 5.0 77.0 5.0 1.120 0.032 HARPS-N 2458503.37914022 39506.8 1.5 6904.6 2.9 71.5 2.9 1.183 0.015 HARPS-N 2458503.37914022 39506.8 1.5 6904.6 2.9 71.5 2.9 1.183 0.015 HARPS-N 2458504.43989909 39509.9 2.4 6912.6 4.8 81.1 4.8 1.114 0.029 HARPS-N 2458504.43989909 39509.9 2.4 6912.6 4.8 81.1 4.8 1.114 0.029 HARPS-N 2458505.38129467 39506.6 1.7 6905.6 3.3 72.6 3.3 1.200 0.019 HARPS-N 2458505.38129467 39506.6 1.7 6905.6 3.3 72.6 3.3 1.200 0.019 HARPS-N 2458505.38129467 39506.6 1.7 6905.6 3.3 72.6 3.3 1.200 0.019 HARPS-N 2458505.38129467 39506.6 1.7 6905.6 3.3 72.6 3.3 1.200 0.019 HARPS-N 2458505.38129467 39506.6 1.7 6905.6 3.3 72.6 3.3 1.200 0.019 HARPS-N 2458505.38129467 39506.6 1.7 6905.6 3.3 72.6 3.3 1.200 0.019 HARPS-N 2458505.38129467 39506.6 1.7 6905.6 3.3 72.6 3.3 1.200 0.019 HARPS-N 2458505.38129467 39506.5 2.1 6915.0 4.2 70.0 4.2 1.102 0.025 HARPS-N 2458518.45830362 39515.6 4.3 6909.7 4.7 77.7 4.7 1.118 0.030 HARPS-N 2458518.45830362 39515.6 4.3 6909.7 4.7 77.7 4.7 1.118 0.000 HARPS-N 2458518.45830362 39515.6 4.3 6909.7 4.7 77.9 84.8 7.0 1.213 0.055 HARPS-N 2458518.45830362 39595.5 2.2 6898.8 4.5										
2458483.48217046         39506.5         1.4         6892.5         2.8         66.2         2.8         1.120         0.013         HARPS-N           2458483.57932245         39507.8         1.3         6886.6         2.6         70.6         2.6         1.118         0.012         HARPS-N           2458484.5739679         39506.9         1.8         6894.0         3.6         61.6         3.6         1.160         0.020         HARPS-N           245848.56813502         39505.3         2.0         6905.7         4.1         75.7         4.1         1.221         0.015         HARPS-N           245848.65813502         39505.3         2.0         6905.7         4.1         75.7         4.1         1.221         0.015         HARPS-N           2458487.5454800         39501.7         1.4         6890.3         2.8         69.1         2.8         1.192         0.015         HARPS-N           2458487.5454800         39497.3         1.2         6901.9         2.5         66.8         2.5         1.138         0.012         HARPS-N           2458488.52873713         39496.3         1.8         6899.7         3.6         70.6         3.6         1.193         0.021         HARPS-N<										
2458483.57932245 39507.8 1.3 6886.6 2.6 70.6 2.6 1.118 0.012 HARPS-N 2458484.45739679 39506.9 1.8 6894.0 3.6 60.6 3.6 1.160 0.020 HARPS-N 2458484.56221664 39507.2 1.5 6892.7 2.9 71.3 2.9 1.127 0.015 HARPS-N 2458486.56813502 39505.3 2.0 6905.7 4.1 75.7 4.1 1.221 0.027 HARPS-N 2458486.56813502 39505.3 2.0 6905.7 4.1 75.7 4.1 1.221 0.027 HARPS-N 2458487.54451438 39500.6 1.4 6899.3 2.8 69.1 2.8 1.192 0.015 HARPS-N 2458487.55454800 39501.7 1.4 6901.2 2.8 69.6 2.8 1.170 0.015 HARPS-N 2458488.41884010 39497.3 1.2 6901.9 2.5 66.8 2.5 1.138 0.012 HARPS-N 2458488.52873713 39499.6 1.9 6900.0 3.9 66.3 3.9 1.206 0.024 HARPS-N 2458489.4534717 39496.3 1.8 6899.7 3.6 70.6 3.6 1.193 0.021 HARPS-N 2458489.58136198 39492.8 1.6 6908.5 3.1 67.7 3.1 1.166 0.018 HARPS-N 2458502.38887026 39505.0 1.7 6903.9 3.3 66.2 3.3 1.123 0.018 HARPS-N 2458502.3893777 39505.4 2.5 6896.3 5.0 77.0 5.0 1.120 0.032 HARPS-N 2458503.37914022 39506.8 1.5 6904.6 2.9 71.5 2.9 1.183 0.012 HARPS-N 2458504.43989909 39509.9 2.4 6912.6 4.8 81.1 4.8 1.114 0.029 HARPS-N 2458504.55233098 39503.5 2.1 6913.6 4.8 81.1 4.8 1.114 0.029 HARPS-N 2458504.55233098 39503.5 2.1 6915.0 4.2 70.0 4.2 1.102 0.025 HARPS-N 2458504.55233098 39503.5 2.1 6915.0 4.2 70.0 4.2 1.102 0.025 HARPS-N 2458504.5849305.5 2.1 6915.0 4.2 70.0 4.2 1.102 0.025 HARPS-N 2458505.38129467 39500.6 1.7 6905.6 3.3 72.6 3.3 1.200 0.019 HARPS-N 2458506.38129467 39500.6 1.7 6905.6 3.3 72.6 3.3 1.200 0.019 HARPS-N 2458506.38129467 39500.6 1.7 6905.6 3.3 72.6 3.3 1.200 0.019 HARPS-N 2458506.38129467 39500.6 1.7 6905.6 3.3 72.6 3.3 1.200 0.019 HARPS-N 2458506.38129467 39500.6 1.7 6905.6 3.3 72.6 3.3 1.200 0.019 HARPS-N 2458506.38129467 39500.6 1.7 6905.6 3.3 72.6 3.3 1.200 0.019 HARPS-N 2458506.36962284 39493.9 3.6 6916.2 7.1 66.2 7.1 1.243 0.055 HARPS-N 2458518.45830362 3915.6 4.3 6932.0 8.7 7.7 7.7 4.7 1.118 0.000 HARPS-N 2458518.45830362 39493.1 1.5 6921.3 7.0 84.8 7.0 1.213 0.055 HARPS-N 2458518.45830362 39493.1 1.5 6893.6 6916.2 7.1 66.2 7.1 1.243 0.055 HARPS-N 2458519.35187655 39498.8 3.8 6910.8 7.7 74.4										
2458484.45739679 39506.9 1.8 6894.0 3.6 61.6 3.6 1.160 0.020 HARPS-N 2458484.56221664 39507.2 1.5 6892.7 2.9 71.3 2.9 1.127 0.015 HARPS-N 2458484.56813502 39505.3 2.0 6905.7 4.1 75.7 4.1 1.221 0.027 HARPS-N 2458487.44451438 39500.6 1.4 6899.3 2.8 69.1 2.8 1.192 0.015 HARPS-N 2458487.5454800 39501.7 1.4 6901.2 2.8 69.6 2.8 1.170 0.015 HARPS-N 2458488.41884010 39497.3 1.2 6901.9 2.5 66.8 2.5 1.138 0.012 HARPS-N 2458488.52873713 39499.6 1.9 6900.0 3.9 66.3 3.9 1.206 0.024 HARPS-N 2458489.45534713 39499.6 1.9 6900.0 3.9 66.3 3.9 1.206 0.024 HARPS-N 2458489.54534717 39496.3 1.8 6899.7 3.6 70.6 3.6 1.193 0.021 HARPS-N 2458502.38887026 39505.0 1.7 6903.9 3.3 66.2 3.3 1.123 0.018 HARPS-N 2458502.38887026 39505.0 1.7 6903.9 3.3 66.2 3.3 1.123 0.018 HARPS-N 2458503.59487143 39505.3 1.2 6903.0 2.5 74.4 2.5 1.170 0.012 HARPS-N 2458503.50487143 39505.3 1.2 6903.0 2.5 74.4 2.5 1.170 0.012 HARPS-N 2458504.4398990 39509.9 2.4 6912.6 4.8 81.1 4.8 1.114 0.029 HARPS-N 2458504.55233098 39503.5 2.1 6915.0 4.2 70.0 4.2 1.102 0.025 HARPS-N 2458505.49840229 39498.6 2.3 6909.7 4.7 77.7 4.7 1.118 0.030 HARPS-N 2458505.49840229 39498.6 2.3 6909.7 4.7 77.7 4.7 1.118 0.030 HARPS-N 2458505.49840229 39498.6 2.3 6909.7 4.7 77.7 4.7 1.118 0.030 HARPS-N 2458505.49840229 39498.6 2.3 6909.7 4.7 77.7 4.7 1.118 0.030 HARPS-N 2458505.49840229 39498.6 2.3 6909.8 4.3 66.3 4.3 1.193 0.027 HARPS-N 2458518.37653154 39505.5 2.2 6909.8 4.3 66.3 4.3 1.193 0.027 HARPS-N 2458518.37653154 39505.5 2.2 6909.8 4.3 66.3 4.3 1.193 0.027 HARPS-N 2458518.37653154 39505.5 2.2 6909.8 4.3 66.3 4.3 1.193 0.027 HARPS-N 2458518.37653154 39505.4 3.5 6921.3 7.0 84.8 7.7 7.4 7 1.120 0.061 HARPS-N 2458519.35187655 39488.8 2.9 6899.0 5.8 7.7 8.4 7.7 1.120 0.061 HARPS-N 2458519.35187655 39498.8 3.8 6910.8 7.7 74.4 7.7 1.120 0.061 HARPS-N 2458519.35187655 39498.8 3.8 6910.8 7.7 74.4 7.7 1.120 0.061 HARPS-N 2458519.35187655 39498.8 3.8 6910.8 7.7 74.4 7.7 1.120 0.061 HARPS-N 2458519.35187655 39498.8 3.8 6910.8 7.7 74.4 7.7 1.120 0.061 HARPS-N 2458519.35187655 39498.8 3.8 6910.8 7.										
2458486.56813502 39505.3 2.0 6905.7 4.1 75.7 4.1 1.221 0.027 HARPS-N 2458487.44451438 39500.6 1.4 6899.3 2.8 69.1 2.8 1.192 0.015 HARPS-N 2458487.55454800 39501.7 1.4 6901.2 2.8 69.6 2.8 1.170 0.015 HARPS-N 2458488.41884010 39497.3 1.2 6901.9 2.5 66.8 2.5 1.138 0.012 HARPS-N 2458488.52873713 39499.6 1.9 6900.0 3.9 66.3 3.9 1.206 0.024 HARPS-N 2458489.43534717 39496.3 1.8 6899.7 3.6 70.6 3.6 1.193 0.021 HARPS-N 2458489.43534717 39496.3 1.8 6899.7 3.6 70.6 3.6 1.193 0.021 HARPS-N 2458489.58136198 39492.8 1.6 6908.5 3.1 67.7 3.1 1.166 0.018 HARPS-N 2458502.38887026 39505.0 1.7 6903.9 3.3 66.2 3.3 1.123 0.018 HARPS-N 2458503.59487143 39505.4 2.5 6896.3 5.0 77.0 5.0 1.120 0.032 HARPS-N 2458503.50487143 39505.3 1.2 6903.0 2.5 74.4 2.5 1.170 0.012 HARPS-N 2458504.43989909 39509.9 2.4 6912.6 4.8 81.1 4.8 1.114 0.029 HARPS-N 2458504.43989909 39509.9 2.4 6912.6 4.8 81.1 4.8 1.114 0.029 HARPS-N 2458505.38129467 39500.6 1.7 6905.6 3.3 72.6 3.3 1.200 0.019 HARPS-N 2458505.38129467 39500.6 1.7 6905.6 3.3 72.6 3.3 1.200 0.019 HARPS-N 2458505.38129467 39500.6 1.7 6905.6 3.3 72.6 3.3 1.200 0.019 HARPS-N 2458505.49840229 39498.6 2.3 6909.7 4.7 77.7 4.7 1.118 0.030 HARPS-N 2458506.56072836 39488.8 2.9 6899.0 5.8 71.8 5.8 1.171 0.041 HARPS-N 2458518.45830362 39515.6 4.3 6932.0 8.7 73.9 8.7 1.278 0.072 HARPS-N 2458518.45830362 39515.6 4.3 6932.0 8.7 73.9 8.7 1.278 0.072 HARPS-N 2458518.45830362 39515.6 4.3 6932.0 8.7 73.9 8.7 1.278 0.072 HARPS-N 2458519.4500523 3950.4 3.5 6932.0 8.7 73.9 8.7 1.278 0.072 HARPS-N 2458519.4500523 3950.4 3.5 6932.0 8.7 73.9 8.7 1.278 0.072 HARPS-N 2458519.4500523 39498.8 3.8 6910.8 7.7 74.4 7.7 1.120 0.061 HARPS-N 2458519.4500523 39494.5 1.8 6914.5 5.5 72.8 3.5 1.157 0.021 HARPS-N 2458520.35461693 39494.5 1.8 6914.5 5.5 72.8 3.5 1.157 0.021 HARPS-N 2458521.4822747 39498.2 2.1 6899.6 4.2 71.1 4.2 1.147 0.027 HARPS-N 2458521.4822747 39498.2 2.1 6899.6 4.2 71.1 4.2 1.147 0.027 HARPS-N 2458521.4822747 39498.2 2.1 6899.6 4.2 71.1 4.2 1.147 0.021 HARPS-N 2458522.43817942 39500.6 1.4 6892.8 2.8 67.9 2.8 1.130							3.6	1.160		
2458487.44451438         3950.6         1.4         6899.3         2.8         69.1         2.8         1.192         0.015         HARPS-N           2458487.55454800         39501.7         1.4         6901.2         2.8         69.6         2.8         1.170         0.015         HARPS-N           2458488.41884010         39497.3         1.2         6901.9         2.5         66.8         2.5         1.138         0.012         HARPS-N           2458488.52873713         39496.6         1.9         6900.0         3.9         66.3         3.9         1.206         0.024         HARPS-N           2458489.43534717         39496.3         1.8         6899.7         3.6         70.6         3.6         1.193         0.021         HARPS-N           2458502.38887026         39505.0         1.7         6903.9         3.3         66.2         3.3         1.123         0.018         HARPS-N           2458502.53993777         39505.4         2.5         6896.3         5.0         77.0         5.0         1.120         0.032         HARPS-N           2458503.50487143         39505.3         1.2         6903.0         2.5         74.4         2.5         1.170         0.012         HARP	2458484.56221664	39507.2	1.5	6892.7	2.9	71.3	2.9	1.127	0.015	HARPS-N
2458487.55454800         39501.7         1.4         6901.2         2.8         69.6         2.8         1.170         0.015         HARPS-N           2458488.41884010         39497.3         1.2         6901.9         2.5         66.8         2.5         1.138         0.012         HARPS-N           2458488.52873713         39499.6         1.9         6900.0         3.9         66.3         3.9         1.206         0.024         HARPS-N           2458489.58136198         39490.3         1.8         6899.7         3.6         70.6         3.6         1.193         0.021         HARPS-N           2458502.38887026         39505.0         1.7         6903.9         3.3         66.2         3.3         1.120         0.032         HARPS-N           2458502.53993777         39506.8         1.5         6904.6         2.9         71.5         2.9         1.183         0.015         HARPS-N           2458503.50487143         39505.3         1.2         6903.0         2.5         74.4         2.5         1.170         0.012         HARPS-N           2458504.5233998         39509.9         2.4         6912.6         4.8         81.1         4.8         1.114         0.029         HARP			2.0						0.027	
2458488.41884010         39497.3         1.2         6901.9         2.5         66.8         2.5         1.138         0.012         HARPS-N           2458488.52873713         39499.6         1.9         6900.0         3.9         66.3         3.9         1.206         0.024         HARPS-N           2458489.43534717         39496.3         1.8         6899.7         3.6         70.6         3.6         1.193         0.021         HARPS-N           2458489.58136198         39492.8         1.6         6908.5         3.1         67.7         3.1         1.166         0.018         HARPS-N           2458502.38887026         39505.0         1.7         6903.9         3.3         66.2         3.3         1.123         0.018         HARPS-N           2458503.37914022         39506.8         1.5         6904.6         2.9         71.5         2.9         1.183         0.015         HARPS-N           2458504.3934777         39505.3         1.2         6903.0         2.5         74.4         2.5         1.170         0.012         HARPS-N           2458504.5923098         39503.5         2.1         6912.6         4.8         81.1         4.8         1.114         0.029         HARPS										
2458488.52873713         39499.6         1.9         6900.0         3.9         66.3         3.9         1.206         0.024         HARPS-N           2458489.43534717         39496.3         1.8         6899.7         3.6         70.6         3.6         1.193         0.021         HARPS-N           2458489.58136198         39492.8         1.6         6908.5         3.1         67.7         3.1         1.166         0.018         HARPS-N           2458502.38887026         39505.0         1.7         6903.9         3.3         66.2         3.3         1.123         0.018         HARPS-N           2458502.3993777         39505.4         2.5         6896.3         5.0         77.0         5.0         1.120         0.032         HARPS-N           2458503.30487143         39505.5         1.2         6903.0         2.5         74.4         2.5         1.170         0.012         HARPS-N           2458504.43989909         39509.9         2.4         6912.6         4.8         81.1         4.8         1.114         0.029         HARPS-N           2458505.38129467         39500.6         1.7         6905.6         3.3         72.6         3.3         1.200         0.019         HARP										
2458489.45534717         39496.3         1.8         6899.7         3.6         70.6         3.6         1.193         0.021         HARPS-N           2458489.58136198         39492.8         1.6         6908.5         3.1         67.7         3.1         1.166         0.018         HARPS-N           2458502.38887026         39505.0         1.7         6903.9         3.3         66.2         3.3         1.123         0.018         HARPS-N           2458503.37914022         39506.8         1.5         6904.6         2.9         71.5         2.9         1.183         0.015         HARPS-N           2458503.50487143         39505.3         1.2         6903.0         2.5         74.4         2.5         1.170         0.012         HARPS-N           2458504.43989909         39509.9         2.4         6912.6         4.8         81.1         4.8         1.114         0.029         HARPS-N           2458505.38129467         39500.6         1.7         6905.6         3.3         72.6         3.3         1.200         0.025         HARPS-N           2458505.49840229         39498.6         2.3         6909.7         4.7         77.7         4.7         1.118         0.030         HAR										HARPS-N
2458489.58136198         39492.8         1.6         6908.5         3.1         67.7         3.1         1.166         0.018         HARPS-N           2458502.38887026         39505.0         1.7         6903.9         3.3         66.2         3.3         1.123         0.018         HARPS-N           2458502.53993777         39505.4         2.5         6896.3         5.0         77.0         5.0         1.120         0.032         HARPS-N           2458503.37914022         39506.8         1.5         6904.6         2.9         71.5         2.9         1.183         0.015         HARPS-N           2458504.43989909         39509.9         2.4         6912.6         4.8         81.1         4.8         1.114         0.029         HARPS-N           2458504.43989909         39509.5         2.1         6915.0         4.2         70.0         4.2         1.102         0.025         HARPS-N           2458505.38129467         39500.6         1.7         6905.6         3.3         72.6         3.3         1.200         0.019         HARPS-N           2458506.49840229         39498.6         2.3         6909.7         4.7         77.7         4.7         1.118         0.030         HAR										
2458502.38887026       39505.0       1.7       6903.9       3.3       66.2       3.3       1.123       0.018       HARPS-N         2458502.53993777       39505.4       2.5       6896.3       5.0       77.0       5.0       1.120       0.032       HARPS-N         2458503.37914022       39506.8       1.5       6904.6       2.9       71.5       2.9       1.183       0.015       HARPS-N         2458503.50487143       39505.3       1.2       6903.0       2.5       74.4       2.5       1.170       0.012       HARPS-N         2458504.43989909       39509.9       2.4       6912.6       4.8       81.1       4.8       1.114       0.029       HARPS-N         2458504.5233098       39503.5       2.1       6915.0       4.2       70.0       4.2       1.102       0.025       HARPS-N         2458505.38129467       39500.6       1.7       6905.6       3.3       72.6       3.3       1.200       0.019       HARPS-N         2458506.36962284       39493.9       3.6       6916.2       7.1       66.2       7.1       1.1243       0.055       HARPS-N         2458518.476330362       39515.6       4.3       6992.0       8.7			-							
2458502.53993777         39505.4         2.5         6896.3         5.0         77.0         5.0         1.120         0.032         HARPS-N           2458503.37914022         39506.8         1.5         6904.6         2.9         71.5         2.9         1.183         0.015         HARPS-N           2458503.50487143         39505.3         1.2         6903.0         2.5         74.4         2.5         1.170         0.012         HARPS-N           2458504.43989909         39509.9         2.4         6912.6         4.8         81.1         4.8         1.114         0.029         HARPS-N           2458504.55233098         39503.5         2.1         6915.0         4.2         70.0         4.2         1.102         0.025         HARPS-N           2458505.38129467         39500.6         1.7         6905.6         3.3         72.6         3.3         1.200         0.019         HARPS-N           2458505.38129467         39500.6         1.7         6905.6         3.3         72.6         3.3         1.200         0.019         HARPS-N           2458506.36962284         3949.8         3.6         6916.2         7.1         66.2         7.1         1.1243         0.055         HAR										
2458503.37914022         39506.8         1.5         6904.6         2.9         71.5         2.9         1.183         0.015         HARPS-N           2458503.50487143         39505.3         1.2         6903.0         2.5         74.4         2.5         1.170         0.012         HARPS-N           2458504.43989909         39509.9         2.4         6912.6         4.8         81.1         4.8         1.114         0.029         HARPS-N           2458504.5233098         39503.5         2.1         6915.0         4.2         70.0         4.2         1.102         0.025         HARPS-N           2458505.38129467         39500.6         1.7         6905.6         3.3         72.6         3.3         1.200         0.019         HARPS-N           2458505.49840229         39498.6         2.3         6909.7         4.7         77.7         4.7         1.118         0.030         HARPS-N           2458506.36962284         39493.9         3.6         6916.2         7.1         66.2         7.1         1.243         0.055         HARPS-N           2458518.37653154         39508.5         2.2         6909.8         4.3         66.3         4.3         1.193         0.027         HARP										
2458503.50487143         39505.3         1.2         6903.0         2.5         74.4         2.5         1.170         0.012         HARPS-N           2458504.43989909         39509.9         2.4         6912.6         4.8         81.1         4.8         1.114         0.029         HARPS-N           2458504.55233098         39503.5         2.1         6915.0         4.2         70.0         4.2         1.102         0.025         HARPS-N           2458505.38129467         39500.6         1.7         6905.6         3.3         72.6         3.3         1.200         0.019         HARPS-N           2458505.49840229         39498.6         2.3         6909.7         4.7         77.7         4.7         1.118         0.030         HARPS-N           2458506.36962284         39493.9         3.6         6916.2         7.1         66.2         7.1         1.243         0.055         HARPS-N           2458506.50672836         39488.8         2.9         6899.0         5.8         71.8         5.8         1.171         0.041         HARPS-N           2458518.47653154         39508.5         2.2         6909.8         4.3         66.3         4.3         1.193         0.027         HAR										
2458504.43989909       39509.9       2.4       6912.6       4.8       81.1       4.8       1.114       0.029       HARPS-N         2458504.5523098       39503.5       2.1       6915.0       4.2       70.0       4.2       1.102       0.025       HARPS-N         2458505.38129467       39500.6       1.7       6905.6       3.3       72.6       3.3       1.200       0.019       HARPS-N         2458505.49840229       39498.6       2.3       6909.7       4.7       77.7       4.7       1.118       0.030       HARPS-N         2458506.36962284       39493.9       3.6       6916.2       7.1       66.2       7.1       1.243       0.055       HARPS-N         2458506.50672836       39488.8       2.9       6899.0       5.8       71.8       5.8       1.171       0.041       HARPS-N         2458518.37653154       39508.5       2.2       6909.8       4.3       66.3       4.3       1.193       0.027       HARPS-N         2458518.47977117       39509.4       2.8       6914.6       5.5       76.9       5.5       1.203       0.040       HARPS-N         2458519.35187655       39498.8       3.8       6910.8       7.7       <										
2458504.55233098       39503.5       2.1       6915.0       4.2       70.0       4.2       1.102       0.025       HARPS-N         2458505.38129467       39500.6       1.7       6905.6       3.3       72.6       3.3       1.200       0.019       HARPS-N         2458505.49840229       39498.6       2.3       6909.7       4.7       77.7       4.7       1.118       0.030       HARPS-N         2458506.36962284       39493.9       3.6       6916.2       7.1       66.2       7.1       1.243       0.055       HARPS-N         2458506.50672836       39488.8       2.9       6899.0       5.8       71.8       5.8       1.171       0.041       HARPS-N         2458518.37653154       39508.5       2.2       6909.8       4.3       66.3       4.3       1.193       0.027       HARPS-N         2458518.45830362       39515.6       4.3       6932.0       8.7       73.9       8.7       1.278       0.072       HARPS-N         2458518.47977117       39509.4       2.8       6914.6       5.5       76.9       5.5       1.203       0.040       HARPS-N         2458519.45005233       39502.4       3.5       6921.3       7.0										
2458505.49840229         39498.6         2.3         6909.7         4.7         77.7         4.7         1.118         0.030         HARPS-N           2458506.36962284         39493.9         3.6         6916.2         7.1         66.2         7.1         1.243         0.055         HARPS-N           2458506.50672836         39488.8         2.9         6899.0         5.8         71.8         5.8         1.171         0.041         HARPS-N           2458518.37653154         39508.5         2.2         6909.8         4.3         66.3         4.3         1.193         0.027         HARPS-N           2458518.45830362         39515.6         4.3         6932.0         8.7         73.9         8.7         1.278         0.072         HARPS-N           2458518.47977117         39509.4         2.8         6914.6         5.5         76.9         5.5         1.203         0.040         HARPS-N           2458519.35187655         39498.8         3.8         6910.8         7.7         74.4         7.7         1.120         0.061         HARPS-N           2458519.3519.45005233         39502.4         3.5         6921.3         7.0         84.8         7.0         1.213         0.055 <t< td=""><td></td><td></td><td>2.1</td><td></td><td>4.2</td><td>70.0</td><td>4.2</td><td>1.102</td><td>0.025</td><td>HARPS-N</td></t<>			2.1		4.2	70.0	4.2	1.102	0.025	HARPS-N
2458506.36962284       39493.9       3.6       6916.2       7.1       66.2       7.1       1.243       0.055       HARPS-N         2458506.50672836       39488.8       2.9       6899.0       5.8       71.8       5.8       1.171       0.041       HARPS-N         2458518.37653154       39508.5       2.2       6909.8       4.3       66.3       4.3       1.193       0.027       HARPS-N         2458518.45830362       39515.6       4.3       6932.0       8.7       73.9       8.7       1.278       0.072       HARPS-N         2458518.47977117       39509.4       2.8       6914.6       5.5       76.9       5.5       1.203       0.040       HARPS-N         2458519.35187655       39498.8       3.8       6910.8       7.7       74.4       7.7       1.120       0.061       HARPS-N         2458519.45005233       39502.4       3.5       6921.3       7.0       84.8       7.0       1.213       0.055       HARPS-N         2458520.35461693       39497.1       1.5       6893.9       2.9       74.7       2.9       1.142       0.015       HARPS-N         2458521.40212719       39499.0       2.2       6889.8       4.5										
2458506.50672836         39488.8         2.9         6899.0         5.8         71.8         5.8         1.171         0.041         HARPS-N           2458518.37653154         39508.5         2.2         6909.8         4.3         66.3         4.3         1.193         0.027         HARPS-N           2458518.45830362         39515.6         4.3         6932.0         8.7         73.9         8.7         1.278         0.072         HARPS-N           2458518.47977117         39509.4         2.8         6914.6         5.5         76.9         5.5         1.203         0.040         HARPS-N           2458519.35187655         39498.8         3.8         6910.8         7.7         74.4         7.7         1.120         0.061         HARPS-N           2458519.45005233         39502.4         3.5         6921.3         7.0         84.8         7.0         1.213         0.055         HARPS-N           2458520.35461693         39497.1         1.5         6893.9         2.9         74.7         2.9         1.142         0.015         HARPS-N           2458521.40212719         39499.0         2.2         6889.8         4.5         71.3         4.5         1.183         0.029         HAR										
2458518.37653154       39508.5       2.2       6909.8       4.3       66.3       4.3       1.193       0.027       HARPS-N         2458518.45830362       39515.6       4.3       6932.0       8.7       73.9       8.7       1.278       0.072       HARPS-N         2458518.47977117       39509.4       2.8       6914.6       5.5       76.9       5.5       1.203       0.040       HARPS-N         2458519.35187655       39498.8       3.8       6910.8       7.7       74.4       7.7       1.120       0.061       HARPS-N         2458519.45005233       39502.4       3.5       6921.3       7.0       84.8       7.0       1.213       0.055       HARPS-N         2458520.35461693       39497.1       1.5       6893.9       2.9       74.7       2.9       1.142       0.015       HARPS-N         2458520.45526091       39494.5       1.8       6914.5       3.5       72.8       3.5       1.157       0.021       HARPS-N         2458521.40212719       39499.0       2.2       6889.8       4.5       71.3       4.5       1.183       0.029       HARPS-N         2458522.35495354       39499.9       1.2       6887.3       2.4										
2458518.45830362       39515.6       4.3       6932.0       8.7       73.9       8.7       1.278       0.072       HARPS-N         2458518.47977117       39509.4       2.8       6914.6       5.5       76.9       5.5       1.203       0.040       HARPS-N         2458519.35187655       39498.8       3.8       6910.8       7.7       74.4       7.7       1.120       0.061       HARPS-N         2458519.45005233       39502.4       3.5       6921.3       7.0       84.8       7.0       1.213       0.055       HARPS-N         2458520.35461693       39497.1       1.5       6893.9       2.9       74.7       2.9       1.142       0.015       HARPS-N         2458520.45526091       39494.5       1.8       6914.5       3.5       72.8       3.5       1.157       0.021       HARPS-N         2458521.49212719       39499.0       2.2       6889.8       4.5       71.3       4.5       1.183       0.029       HARPS-N         2458522.35495354       39499.9       1.2       6887.3       2.4       65.3       2.4       1.132       0.011       HARPS-N         2458728.243817942       39499.17       0.89       6953.5       1.8										
2458518.47977117       39509.4       2.8       6914.6       5.5       76.9       5.5       1.203       0.040       HARPS-N         2458519.35187655       39498.8       3.8       6910.8       7.7       74.4       7.7       1.120       0.061       HARPS-N         2458519.45005233       39502.4       3.5       6921.3       7.0       84.8       7.0       1.213       0.055       HARPS-N         2458520.35461693       39497.1       1.5       6893.9       2.9       74.7       2.9       1.142       0.015       HARPS-N         2458520.45526091       39494.5       1.8       6914.5       3.5       72.8       3.5       1.157       0.021       HARPS-N         2458521.40212719       39499.0       2.2       6889.8       4.5       71.3       4.5       1.183       0.029       HARPS-N         2458521.48828747       39498.2       2.1       6899.6       4.2       71.1       4.2       1.147       0.027       HARPS-N         2458522.35495354       39499.9       1.2       6887.3       2.4       65.3       2.4       1.132       0.011       HARPS-N         2458522.43817942       39500.6       1.4       6892.8       2.8										
2458519.35187655       39498.8       3.8       6910.8       7.7       74.4       7.7       1.120       0.061       HARPS-N         2458519.45005233       39502.4       3.5       6921.3       7.0       84.8       7.0       1.213       0.055       HARPS-N         2458520.35461693       39497.1       1.5       6893.9       2.9       74.7       2.9       1.142       0.015       HARPS-N         2458520.45526091       39494.5       1.8       6914.5       3.5       72.8       3.5       1.157       0.021       HARPS-N         2458521.40212719       39499.0       2.2       6889.8       4.5       71.3       4.5       1.183       0.029       HARPS-N         2458521.48828747       39498.2       2.1       6899.6       4.2       71.1       4.2       1.147       0.027       HARPS-N         2458522.35495354       39499.9       1.2       6887.3       2.4       65.3       2.4       1.132       0.011       HARPS-N         2458522.43817942       39500.6       1.4       6892.8       2.8       67.9       2.8       1.130       0.015       HARPS-N         2458788.78775712       39499.17       0.89       6953.5       1.8										
2458519.45005233       39502.4       3.5       6921.3       7.0       84.8       7.0       1.213       0.055       HARPS-N         2458520.35461693       39497.1       1.5       6893.9       2.9       74.7       2.9       1.142       0.015       HARPS-N         2458520.45526091       39494.5       1.8       6914.5       3.5       72.8       3.5       1.157       0.021       HARPS-N         2458521.40212719       39499.0       2.2       6889.8       4.5       71.3       4.5       1.183       0.029       HARPS-N         2458521.48828747       39498.2       2.1       6899.6       4.2       71.1       4.2       1.147       0.027       HARPS-N         2458522.35495354       39499.9       1.2       6887.3       2.4       65.3       2.4       1.132       0.011       HARPS-N         2458522.43817942       39500.6       1.4       6892.8       2.8       67.9       2.8       1.130       0.015       HARPS-N         2458788.78775712       39499.17       0.89       6953.5       1.8       43.7       1.8       1.1403       0.0020       ESPRESSO										
2458520.35461693       39497.1       1.5       6893.9       2.9       74.7       2.9       1.142       0.015       HARPS-N         2458520.45526091       39494.5       1.8       6914.5       3.5       72.8       3.5       1.157       0.021       HARPS-N         2458521.40212719       39499.0       2.2       6889.8       4.5       71.3       4.5       1.183       0.029       HARPS-N         2458521.48828747       39498.2       2.1       6899.6       4.2       71.1       4.2       1.147       0.027       HARPS-N         2458522.35495354       39499.9       1.2       6887.3       2.4       65.3       2.4       1.132       0.011       HARPS-N         2458522.43817942       39500.6       1.4       6892.8       2.8       67.9       2.8       1.130       0.015       HARPS-N         2458788.78775712       39499.17       0.89       6953.5       1.8       43.7       1.8       1.1403       0.0020       ESPRESSO										
2458520.45526091     39494.5     1.8     6914.5     3.5     72.8     3.5     1.157     0.021     HARPS-N       2458521.40212719     39499.0     2.2     6889.8     4.5     71.3     4.5     1.183     0.029     HARPS-N       2458521.48828747     39498.2     2.1     6899.6     4.2     71.1     4.2     1.147     0.027     HARPS-N       2458522.35495354     39499.9     1.2     6887.3     2.4     65.3     2.4     1.132     0.011     HARPS-N       2458522.43817942     39500.6     1.4     6892.8     2.8     67.9     2.8     1.130     0.015     HARPS-N       2458788.78775712     39499.17     0.89     6953.5     1.8     43.7     1.8     1.1403     0.0020     ESPRESSO										
2458521.40212719       39499.0       2.2       6889.8       4.5       71.3       4.5       1.183       0.029       HARPS-N         2458521.48828747       39498.2       2.1       6899.6       4.2       71.1       4.2       1.147       0.027       HARPS-N         2458522.35495354       39499.9       1.2       6887.3       2.4       65.3       2.4       1.132       0.011       HARPS-N         2458522.43817942       39500.6       1.4       6892.8       2.8       67.9       2.8       1.130       0.015       HARPS-N         2458788.78775712       39499.17       0.89       6953.5       1.8       43.7       1.8       1.1403       0.0020       ESPRESSO										
2458521.48828747     39498.2     2.1     6899.6     4.2     71.1     4.2     1.147     0.027     HARPS-N       2458522.35495354     39499.9     1.2     6887.3     2.4     65.3     2.4     1.132     0.011     HARPS-N       2458522.43817942     39500.6     1.4     6892.8     2.8     67.9     2.8     1.130     0.015     HARPS-N       2458788.78775712     39499.17     0.89     6953.5     1.8     43.7     1.8     1.1403     0.0020     ESPRESSO										
2458522.35495354       39499.9       1.2       6887.3       2.4       65.3       2.4       1.132       0.011       HARPS-N         2458522.43817942       39500.6       1.4       6892.8       2.8       67.9       2.8       1.130       0.015       HARPS-N         2458788.78775712       39499.17       0.89       6953.5       1.8       43.7       1.8       1.1403       0.0020       ESPRESSO										
2458788.78775712 39499.17 0.89 6953.5 1.8 43.7 1.8 1.1403 0.0020 ESPRESSO		39499.9	1.2	6887.3	2.4	65.3	2.4	1.132	0.011	HARPS-N
2458804.67601741 39480.32 0.67 6965.9 1.3 65.6 1.3 1.2545 0.0013 ESPRESSO										
	2458804.67601741	39480.32	0.67	6965.9	1.3	65.6	1.3	1.2545	0.0013	ESPRESSO

Table 2 (continued)
RV observations and activity indicators

BJD (TDB)	RV	$\sigma_{ m RV}$	CCF BIS	$\sigma_{ m BIS}$	CCF FWHM	$\sigma_{ m FWHM}$	$S_{HK}$	σα	Instrument
Bob (IBB)	$(m s^{-1})$	$(m s^{-1})$	$(m s^{-1})$	$(m s^{-1})$	$(m s^{-1})$	$(m s^{-1})$	$\sim_{HK}$	$\sigma_{ m S_{HK}}$	mon amon
	(III S )	(III S )	(III S )	(III S )	(III S )	(III S )			
2458806.80347928	39484.42	0.79	6928.5	1.6	56.1	1.6	1.0794	0.0016	ESPRESSO
2458808.76852035	39504.65	0.83	6941.7	1.7	41.2	1.7	1.0573	0.0018	ESPRESSO
2458820.76166121	39489.22	0.46	6928.21	0.91	48.14	0.91	1.18743	0.00067	ESPRESSO
2458825.59389775	39492.79	0.71	6962.1	1.4	60.4	1.4	1.1525	0.0014	ESPRESSO
2458833.58700359	39486.65	0.70	6934.8	1.4	54.4	1.4	1.1807	0.0013	ESPRESSO
2458839.65413441	39493.99	0.63	6955.9	1.3	54.1	1.3	1.2941	0.0011	ESPRESSO
2458840.58619720	39501.76	0.70	6967.2	1.4	41.1	1.4	1.3193	0.0013	ESPRESSO
2458848.60085991	39501.35	0.49	6942.72	0.98	43.38	0.98	1.17686	0.00075	ESPRESSO
2458849.56597102	39505.53	0.69	6955.6	1.4	38.6	1.4	1.1913	0.0013	ESPRESSO
2458850.58225768	39494.9	1.8	6972.4	3.5	46.6	3.5	1.2761	0.0044	ESPRESSO
2458850.60464655	39497.81	0.92	6955.0	1.8	34.1	1.8	1.2108	0.0019	ESPRESSO
2458851.58865177	39493.17	0.79	6953.3	1.6	57.3	1.6	1.2570	0.0016	ESPRESSO
2458853.68186920	39502.19	0.57	6968.8	1.1	58.0	1.1	1.3340	0.0010	ESPRESSO
2458864.55947341	39502.03	0.65	6954.6	1.3	44.6	1.3	1.2129	0.0012	ESPRESSO
2458864.64168610	39502.17	0.77	6944.7	1.5	53.7	1.5	1.2462	0.0017	ESPRESSO
2458865.59784818	39505.73	0.94	6978.3	1.9	38.7	1.9	1.3126	0.0024	ESPRESSO
2458869.61564757	39488.28	0.56	6996.3	1.1	63.6	1.1	1.2687	0.0011	ESPRESSO
2458886.57544506	39481.55	0.69	6924.4	1.4	52.8	1.4	1.2086	0.0013	ESPRESSO
2458887.57037120	39487.19	0.61	6925.7	1.2	45.6	1.2	1.1117	0.0011	ESPRESSO
2458906.52291945	39500.21	0.67	6988.0	1.3	45.9	1.3	1.2254	0.0012	ESPRESSO
2459110.65183858	39492.2	2.7	6957.0	5.3	66.3	5.3	1.251	0.033	HARPS-N
2459111.66733900	39505.2	1.2	6956.5	2.5	67.6	2.5	1.401	0.011	HARPS-N
2459112.66195511	39508.2	1.9	6955.8	3.8	64.1	3.8	1.294	0.020	HARPS-N
2459120.71102749	39512.7	1.3	6979.6	2.7	70.1	2.7	1.339	0.013	HARPS-N
2459153.51589766	39502.7	2.4	6939.2	4.7	67.1	4.7	1.216	0.026	HARPS-N

#### 3.1. Stellar Rotation Period

One parameter of special interest is the stellar rotation period, which we include as a parameter in our RV model (see Section 4.5). M18 conducted a Lomb-Scargle periodogram on the K2 light curve and reported a rotation period of  $15.04 \pm 1.01$  days. Ciardi et al. (2018) analyzed the same light curve and found a rotation period of  $15.2\pm0.2$  days through a Lomb-Scargle periodogram and  $13.8\pm1.0$  days through an autocorrelation function. Livingston et al. (2018) conducted a Gaussian process (GP) regression, a Lomb-Scargle periodogram, and an autocorrelation function on the light curve and found a corresponding rotation period of  $13.5^{+0.7}_{-0.4}$  d,  $15.1^{+1.3}_{-1.2}$  d, and  $13.6^{+2.2}_{-1.5}$  d, respectively. Note: Given an offset and uncertainties in the photometric data set, a generalized Lomb-Scargle periodogram would be preferred (Zechmeister & Kürster 2009); however, it is not clear from the referenced papers whether this generalized method was used or just a basic Lomb-Scargle periodogram (Scargle 1982).

Notably, the estimates via a Lomb-Scargle periodogram are longer than estimates with other methods. All results are broadly consistent with our findings from our full model results  $(13.37^{+0.13}_{-0.17})$  days; see Table 4), except the 15.2±0.2 day result from the Lomb-Scargle analysis by Ciardi et al. (2018). They also have the smallest uncertainties of any rotation period estimate, so it is possible that their value is reasonable but the uncertainties are overly optimistic.

A possible explanation of this discrepancy could be differential rotation. Regardless of activity level, starspots, plage, and other activity may be more prominent at different stellar latitudes when the K2 photometry and our HARPS-N spectroscopy were conducted. This hypothesis is also mentioned by Ciardi et al. (2018) to explain a larger than expected vsin i. Following Barnes et al. (2005) and Kitchatinov & Olemskoy (2012), they estimate that the equatorial rotation period of K2-136

could be faster than higher latitudes by  $\sim 1$  day. Then again, Aigrain et al. (2015) found that claims of differential rotation should be treated with caution even for long baselines of photometry. We may simply be seeing different starspots at different longitudes creating phase modulation, combined with greater or fewer numbers of starspots leading to better or worse constraints on rotation period.

## 3.2. Binarity of K2-136

One of the planet discovery papers, Ciardi et al. (2018), reported a binary companion to K2-136. In addition to their K2 photometric analysis, they collected spectra from the SpeX spectrograph (Rayner et al. 2003, 2004) at the 3-m NASA Infrared Telescope Facility and the HIRES spectrograph (Vogt et al. 1994) at the Keck I telescope, as well as AO observations with the NIRC2 instrument at the Keck II telescope and the P3K AO system and PHARO camera (Hayward et al. 2001) on the 200" Hale Telescope at Palomar Observatory. The AO observations at both facilities detected an M7/8V star separated from the primary star by  $\sim$  0.7", corresponding to a projected separation of ~ 40 AU; the spectroscopic observations did not detect this companion, and no further companions were found by any of the above observations. (Notably, this angular separation is more than enough for HST to resolve; see Sections 4.9 and 2.5.)

Gaia DR3 did not detect the binary companion, leaving the issue of boundedness unresolved. However, Ciardi et al. (2018) compared the current position of K2-136 against observations from the 1950 Palomar Observatory Sky Survey (POSS I) and noted that the star had moved 6" in the intervening time with no evidence of background stars. These POSS I observations show that the stellar companion is likely bound.

Further, Gaia DR3 reported K2-136 to have an astrometric excess noise of 96  $\mu$ as and a Renormalised Unit

Weight Error (RUWE) of 1.23, a mild departure from a good single-star model. At the separation and brightness of the companion, this excess variability in the astrometry is unlikely to be due to pollution from its light contribution: at  $\sim 0.7$ " separation a companion can be detected only with a G magnitude difference of  $\lesssim 2$  (Gaia Collaboration et al. 2021). There is therefore a mild indication of astrometric variability due to unmodeled orbital motion. Using the formalism of Torres (1999), at the distance of the system, given its angular separation, and for the mass range of an M7/8 star, the median astrometric acceleration is expected to be  $\sim 25~\mu \rm as~yr^{-2}$ , with maximum value close to 40  $\mu \rm as~yr^{-2}$ , indicating that in addition to simple astrometric noise, the bulk of the astrometric variability could be caused by the detection of the acceleration due to the companion.

It is worth considering whether flux from the companion could bias the measured RVs of the primary K dwarf. Both the HARPS-N and ESPRESSO band passes are approximately 380nm – 690nm and centered on the V band. According to Ciardi et al. (2018), the M dwarf companion is at least 10 magnitudes fainter than the primary in the V-band. We can use  $\Delta m = 10$  as a worst-case scenario and similarly assume the companion star was well-centered on the fiber for all observations (because the companion and primary are separated by 0.7", the companion would not be well-centered and the actual flux contamination from the companion would be less). Cunha et al. (2013) explored the RV impact of flux contamination from a stellar companion: for a K5 dwarf and an M dwarf (M3 or later) with  $\Delta m = 10$ , the maximum impact on RVs is  $< 10 \text{ cm s}^{-1}$ , and therefore negligible for our level of RV precision.

Ciardi et al. (2018) explored whether the transit signals may originate from the M dwarf. They found that in order to match the observed transit depth of K2-136c, the M dwarf would have to be a binary system itself that exhibits significant and detectable secondary eclipses, which have not been observed. Further, the transit duration of K2-136c is inconsistent with a transit of an M dwarf. Finally, K2-136c has already been validated by Ciardi et al. (2018) and all three planets have been independently validated by M18 and Livingston et al. (2018). Therefore, it is very unlikely that the planets are false positive signals or planetary signals from the M dwarf.

However, in the *Kepler* band pass, the companion M dwarf is 6.5 magnitudes fainter, which leads to a very small dilution effect on the planet transit depths. Following Ciardi et al. (2015), we include this effect for the sake of robustness in our final planet radius estimates (which enlarges each planet by  $\sim 0.13\%$ ).

This binary companion may also cause a long-term RV trend, which we discuss further in Section 4.5 and test in Section 4.10.

## 4. DATA ANALYSIS

We analyzed the RV data in conjunction with a number of other common stellar activity indices that are calculated with the ESPRESSO DRS 2.2.8 pipeline, specifically the CCF BIS, CCF FWHM, and  $S_{HK}$ . In this section, we first explore the data set by generating a periodogram and conducting a correlation analysis between the RVs and other data types. Then we discuss the transit and RV components of our model, the param-

eter estimation process, and how we compare our models. Finally, we conduct tests on our results and discuss the implications of a binary companion in the system.

# 4.1. Periodogram Analysis

In order to investigate periodic signals in our data (planetary or otherwise), we created Generalized Lomb-Scargle periodograms (Scargle 1982; Zechmeister & Kürster 2009) of our RVs and our stellar activity indices. As a point of reference, we also included the window function of our data (built from constant, non-zero values at each of the timestamps of our observations). It is used to determine the regular patterns in the periodograms due to the sampling and gaps in the time series. These periodograms are presented in Fig. 1.

To ascertain the robustness of any apparent signals, we also estimated each periodogram's False Alarm Probability (FAP), the likelihood that an apparent signal of a given strength will be detected when no underlying signal is actually present. The FAP was estimated with the bootstrap method: sampling the observations randomly with replacement while maintaining the same timestamps. We repeat this process 100000 times, each time constructing a periodogram and determining the maximum peak. This reveals how often a given signal strength will appear due only to noise, from which the FAP is calculated.

The strongest RV signals in our combined periodogram (both HARPS-N and ESPRESSO) are at the orbital period of K2-136c, the rotation period of the star, and near  $0.017~\mathrm{d^{-1}}$  (i.e. half the length of the ESPRESSO data baseline of 117.7 days), although none are significant at the 1% level. Among the stellar activity periodograms, the strongest signals are the rotation period signal in the ESPRESSO FWHM power and a long-period signal in the HARPS-N FWHM power which can be attributed to the window function. Also, the strongest peak in the (combined data) window function periodogram above  $0.01 \,\mathrm{days^{-1}}$  (near  $0.03 \,\mathrm{days^{-1}}$ ) does not correspond to any significant signals or aliases in any of the four data types. As for low-frequency signals  $< 0.01 \text{ days}^{-1}$ , we discuss possible long-term trends in Sections 3.2 and 4.5. All of this indicates that K2-136c has a more detectable RV signal than the other two planets, as expected given its size.

## 4.2. Correlation Analysis

We also examined the relationship between RVs and our stellar activity indices. Because RVs are measured from small shifts in spectral absorption lines, and stellar activity can change the shape of absorption lines, stellar activity can significantly affect RV observations (e.g. Queloz et al. 2001; Haywood 2015; Rajpaul et al. 2015). Scatter plots between RVs and all three activity indices are presented in Fig. 2. At least in the case of  $S_{HK}$  and FWHM, there are notable correlations with RVs according to the p-values for the Spearman correlation coefficient (which captures nonlinear, monotonic correlations and uses the same -1 to 1 range as the Pearson correlation coefficient). According to the Spearman coefficient, there is a correlation of 0.26 between RV and  $S_{HK}$ , a negative correlation of -0.18 between RV and BIS, and the strongest correlation of 0.39 between RV and FWHM.

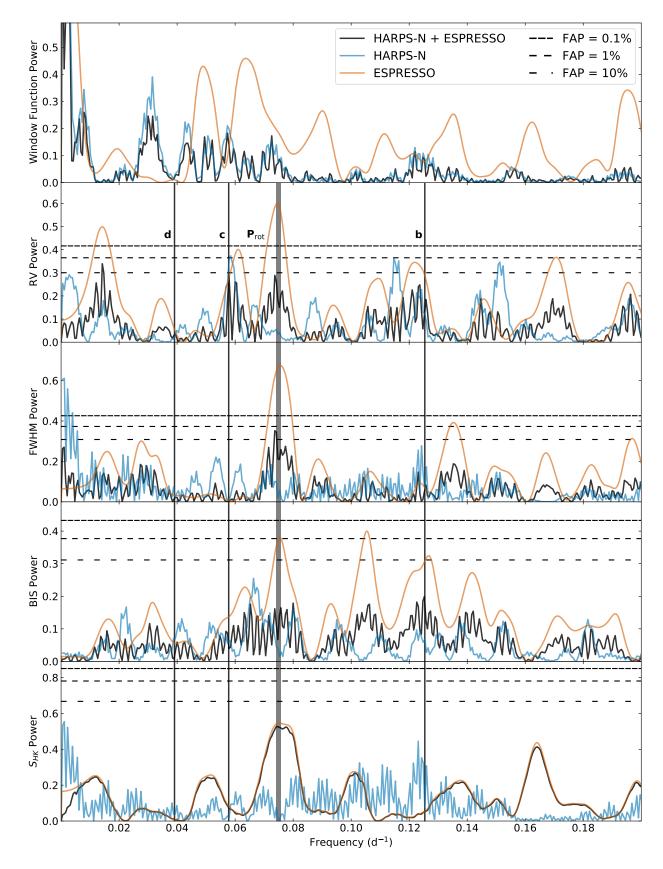


Figure 1. Periodograms of RV, CCF FWHM, CCF BIS, and  $S_{HK}$  for the K2-136 system. In the top panel is the window function (computed from observation times only). Each subplot has the periodogram of HARPS-N and ESPRESSO combined (black), HARPS-N alone (blue), and ESPRESSO alone (orange). The gray region corresponds to the  $1\sigma$  confidence interval of the stellar rotation period (as determined from our model results); the three vertical, black lines correspond to the orbital periods of K2-136b, c, and d. Finally, the horizontal dashed lines refer to different false alarm probabilities (for HARPS-N and ESPRESSO combined).

K2-136c 9

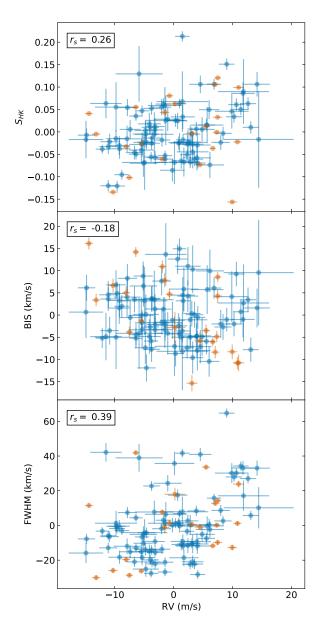


Figure 2. Scatter plots of  $S_{HK}$ , BIS, and FWHM against RV for the K2-136 system. All HARPS-N and ESPRESSO data have been separately offset shifted according to the median model offsets listed in Table 4. Blue data points correspond to HARPS-N observations, orange data points to ESPRESSO. In the top-left corner of each subplot is the Spearman correlation coefficient, which can capture nonlinear, monotonic correlations. (Coefficients were calculated with data values but not uncertainties.)

For a data set of this size, these coefficients correspond to p-values of 0.004 for RV and  $S_{HK}$ , 0.052 for RV and BIS, and  $\ll$  0.001 for RV and FWHM. Therefore, for RV and  $S_{HK}$  and especially RV and FWHM, there appears to be a statistically significant correlation. In other words, there is good reason to believe that this data set includes correlated and structured stellar activity. In fact, the Spearman correlation coefficient is likely an underestimate of the correlation between RVs and stellar activity indices, since there can be a phase shift in the amplitude variation from one data type to another (Santos et al. 2014; Collier Cameron et al. 2019).

## 4.3. K2 Transit Photometry

We cleaned and flattened the photometric data from K2 using the exact same procedure as was used originally in M18. Their procedure follows the self-flatfielding (SFF) method developed in Vanderburg & Johnson (2014) to perform a rough removal of instrumental variability followed by a simultaneous fit to a model consisting of Mandel & Agol (2002) transit shapes for the three planets, a basis spline in time to describe the stellar variability, and splines in Kepler's roll angle to describe the systematic photometric errors introduced by the spacecraft's unstable pointing (Vanderburg et al. 2016). After performing the fit, they removed the best-fit systematics and stellar variability components, isolating the transits for further analysis. The interested reader should refer to M18 for additional detail of the full procedure.

We modeled the flattened and cleaned M18 light curve with the BATMAN Python package (Kreidberg 2015), based on the Mandel & Agol (2002) transit model. Our model included a baseline offset parameter and white noise parameter for our K2 Campaign 13 photometry as well as two quadratic limb-darkening parameters (parameterized using Kipping 2013). Each planet was modeled with five parameters: the transit time, orbital period, planet radius relative to stellar radius, transit duration, and impact parameter. All parameters were modeled with either uniform, Gaussian, Jeffreys, or modified Jeffreys priors (Gregory 2007). Only the photometric white noise parameters used modified Jeffreys priors, with a knee located at the mean of the photometric flux uncertainty for that particular campaign or sector. All priors are listed in Table 3. The raw and flattened data can be seen in Fig. 3.

We also applied a Gaussian prior on stellar density by comparing the spectroscopically derived stellar density to the stellar density found via the following equation (Seager & Mallén-Ornelas 2003; Sozzetti et al. 2007):

$$\rho_* = \frac{3\pi}{GP^2} \left(\frac{a}{R_*}\right)^3 \tag{1}$$

where orbital period (P) and the semi-major axis  $(a/R_*)$  are derived directly from the light curve model.

All together, our full transit model includes 15 planetary parameters (5 per planet: time of transit, orbital period, ratio of planet radius to stellar radius, transit duration, and impact parameter), 2 quadratic limb darkening parameters, 1 photometric noise parameter, and 1 photometric baseline offset parameter for a total of 19 parameters.

The only parameters in common between our transit model and our RV model (as explained in further detail below) are transit times and orbital periods.

# 4.4. TESS Transit Photometry

No pre-processed light curves were available for the TESS Sector 43 observation of K2-136, so we extracted the photometry from the full frame image (FFI) pixel level. Following Vanderburg et al. (2019), we constructed 20 different apertures (10 circular, 10 shaped like the TESS point spread function) and selected the one that best minimized photometric scatter. As for TESS Sector

44 observations, we used the simple aperture photometry (SAP) light curve produced by the Science Processing Operations Center (SPOC) pipeline (Jenkins et al. 2016). Light curves from both sectors were then flattened in the same way: a basis spline fit was performed iteratively on the photometry (with breakpoints every 0.3 days in order to adequately model stellar variability) and  $3\sigma$  outliers were removed until convergence (this too, aside from the breakpoint length, follows Vanderburg et al. 2019). Finally, we conducted a simultaneous fit of the low-frequency variability and the transits in order to determine the best-fit low-frequency variability.

TESS photometry is not incorporated into our final photometric model, although we did run exploratory joint transit models on K2 and TESS photometry simultaneously. The transit signals of the two smaller planets, K2-136b and d were too small to reliably detect in the TESS photometry: individual transits were indistinguishable in depth and quality from temporally adjacent stellar activity. However, the transits of K2-136c were easily identifiable individually in TESS photometry, so we ran a joint transit model on all K2 photometry and TESS photometry to explore the resulting improvements in the parameters of K2-136c. This joint transit model included all parameters listed in Section 4.3 as well as additional baseline offset and white noise parameters for the two TESS Sectors (43 and 44) and two additional quadratic limb-darkening parameters for TESS photometry for six additional parameters total. The fit resulted in consistent values for all planet and system parameters as well as a dramatically more precise ephemeris for K2-136c:  $P_c = 17.307081^{+0.000014}_{-0.000013}$  days and  $t_{0,c} = 8678.07179^{+0.00067}_{-0.00063}$  (BJD-2450000). For comparison, this period and transit time have uncertainties that are that ties that are both approximately 15x tighter than those resulting from K2 transit modeling alone (see Table 3). We report these values here to minimize ephemeris drift and facilitate planning of future transit observations of K2-136c.

## 4.5. RV Model

We modeled the RV signal of the orbiting planets and the stellar activity simultaneously. We assumed non-interacting planets with Keplerian orbits. We used RadVel (Fulton et al. 2018) to model the RV signal from each planet with 5 parameters: reference epoch, orbital period, RV semi-amplitude, eccentricity, and argument of periastron. The latter two parameters, eccentricity and longitude of periastron, were parameterized as  $\sqrt{e}\cos w$ and  $\sqrt{e}\sin w$ . As explained in Eastman et al. (2013), this reparameterization avoids a boundary condition at zero eccentricity that may lead to eccentricity estimates that are systematically biased upward. We conducted trial simulations with circular versus eccentric orbits for all three planets and found excellent agreement in all parameters (less than  $1\sigma$ ). We opted to keep eccentricity and argument of the periastron as parameters in order to constrain or place upper limits on each planet's eccentricity. Additionally, we prevented system configurations that would lead to orbit crossings of any two planets, as well as overlaps of planetary Hill spheres. For each planet's reference epoch and orbital period, we applied a Gaussian prior based on the transit parameters determined from M18. We analyzed the K2 transit photometry with and without TESS photometry and verified these M18 values (see Table 3).

We also applied additional prior limits on the eccentricities of K2-136b and K2-136d. Based on preliminary modeling of all three planets with uninformed prior eccentricity constraints (and everything else identical to our final model), we found that we could determine the eccentricity of K2-136c but not its siblings. Thus, we decided to set eccentricity constraints by using the Stability of Planetary Orbital Configurations Klassifier (SPOCK; Tamayo et al. 2020), an N-body simulator that employs machine learning to improve performance. We input into SPOCK our stellar mass posterior and our orbital period posteriors for all three planets (from our preliminary simulations). We also input the mass, eccentricity, and argument of the periastron posteriors for K2-136c (again, from our early simulations). Lastly, we input uniform distributions for mass, eccentricity, and argument of the periastron for K2-136b and K2-136d. Planet mass ranged from 0 up to that of approximately 100% iron planet composition (3  $M_{\oplus}$  for K2-136b and 30  $M_{\oplus}$  for K2-136d; Fortney et al. 2007). Eccentricity ranged from 0 to 0.6 and argument of the periastron ranged from 0 to 360 degrees. We took the subset of our sample that had a > 90% chance of surviving for  $> 10^9$  orbits (of the innermost planet) and then determined the  $3\sigma$  upper limit on the eccentricities of K2-136b and K2-136d for that subset. We then used those values,  $e_{\rm b,max}=0.35$  and  $e_{\rm d,max}=0.37,$  as eccentricity upper limit priors in all subsequent simulations.

Given the M dwarf companion to our host star (Ciardi et al. 2018), we wanted to include the potential for an RV trend caused by this companion. For further discussion of binarity and linear trends, see Section 3.2. Our planetary RV signals and the RV trend therefore take the following form:

$$RV = \sum_{i \in \{b,c,d\}} K_i \left( \cos \left( \omega_i + f_i \right) + e_i \cos \omega_i \right) + mt \quad (2)$$

$$f = 2\arctan\left(\sqrt{\frac{1+e}{1-e}}\tan\frac{E}{2}\right) \tag{3}$$

$$M = E - e\sin E \tag{4}$$

$$M = nt = \frac{2\pi(t - \tau)}{P} \tag{5}$$

where K is the induced RV semi-amplitude,  $\omega$  is the argument of the periastron, f is the true anomaly, e is the eccentricity, m is the slope of the RV trend, t is the observation time, E is the eccentric anomaly, M is the mean anomaly, n is the mean motion,  $\tau$  is the time of periastron passage (as calculated from transit time, orbital period, eccentricity, and argument of the periastron), and P is the orbital period.

The stellar activity was handled via a GP on RVs. We first used a simultaneous model of stellar activity on four different data types: RV, FWHM (a measure of the width of absorption lines), BIS (a measure of line asymmetry),

and  $S_{HK}$  (an estimate of chromospheric magnetic activity via emission in the cores of the Ca II H & K lines). However, we found that this approach forced the model to include unreasonable amounts of white noise into each data type via a white noise jitter parameter included in our model. Further, it did not lead to a notable improvement in our final parameter constraints. We conducted numerous tests exploring the excess white noise preferred by the model, including modeling different instruments, different numbers of planets, altering the data reduction pipeline (e.g. trying the ZLSD pipeline; Lienhard et al. 2022), and creating synthetic data sets to model against. The most reasonable hypothesis we could find is that for the K2-136, our data (especially for ESPRESSO) is of a sufficiently high quality, with small enough uncertainties, that the model we used from Rajpaul et al. (2015) to relate the stellar activity indices to each other and to the RVs was not complex enough to account for the correlated structure of the stellar activity of K2-136.

Our RV data and the final RV model fit can be seen in Fig. 4. Despite only modeling RVs without any stellar activity indices, a GP is still robust and allows us to separate planet-induced RVs from stellar activity to the extent that disentanglement is possible. We followed the method laid out in Rajpaul et al. (2015), but we constrained the model only to the portions relevant to RVs rather than additional stellar activity indices. They dictate that the RVs are related to the stellar activity as follows:

$$\Delta RV = V_c G(t) + V_r \dot{G}(t) \tag{6}$$

In this equation, G(t) corresponds to the underlying stellar activity GP, while  $V_c$  and  $V_r$  correspond to the RV amplitudes of the convective blueshift and rotation modulation effect, respectively. It is important to include both rotation modulation and convective blueshift for data types impacted by both, as one phenomenon may play a larger role than the other depending on the data type and star. In fact, our final results (see Table 4) show that for K2-136, rotation modulation has an outsized effect on RVs compared to convective blueshift; however, we retain both terms in our model since  $V_c$  is still inconsistent with zero. We follow Rajpaul et al. (2015) further by using a quasi-periodic kernel to establish the covariance matrix of our GP. A quasi-periodic kernel is a good choice to capture the stellar variability of a star because quasi-periodicity describes well the variability exhibited by a rotating star with starspots that come and go. Following Giles et al. (2017), we find a predicted starspot lifetime for K2-136 of  $38^{+20}_{-13}$  days (versus a rotation period of 13.37 days); this estimate is consistent with our GP evolution time-scale result ( $48^{+19}_{-11}$  days, see Table 4). In other words, stellar activity during the time frame of a single rotation period is likely to look similar (though not identical) to stellar activity during the previous and subsequent stellar rotation periods, since the starspots for K2-136 are likely to be longer lived than the stellar rotation period. Thus, the quasi-periodic kernel is defined as follows:

$$K_{\rm QP}(t_i, t_j) = h^2 \exp\left(-\frac{\sin^2\left(\pi(t_i - t_j)/P_*\right)}{2\lambda_p^2} - \frac{(t_i - t_j)^2}{2\lambda_e^2}\right), \quad (7)$$

where h is the GP amplitude (which is folded into the amplitude parameters described above),  $P_*$  is the stellar stellar rotation period,  $\lambda_e$  is a decay timescale proportional to the starspot lifetime, and  $\lambda_p$  is a smoothness parameter that captures the level of variability within a single rotation period.  $t_i$  and  $t_j$  are any two times between which the covariance is being calculated; for a given time series of N observations, all  $N^2$  combinations of time pairs create the NxN covariance matrix. This covariance matrix (plus a mean model) is a normal multivariate distribution; G(t) can be explored by sampling from this distribution. We refer the reader to Rajpaul et al. (2015) for a more detailed description of this method, as well as Mayo et al. (2019) for an application of this method to the sub-Neptune Kepler-538b.

Finally, we include a jitter parameter (added in quadrature to RV uncertainties) and a baseline offset parameter for each instrument (HARPS-N and ESPRESSO). All together, our full model includes 21 planetary parameters (5 per planet: time of transit, orbital period, RV semi-amplitude,  $\sqrt{e}\sin\omega$ , and  $\sqrt{e}\cos\omega$ ), 5 GP parameters (2 GP amplitudes corresponding to  $V_c$  and  $V_r$  from equation 6 as well as  $P_*$ ,  $\lambda_p$ , and  $\lambda_e$  from equation 7), 1 linear trend parameter, 2 RV noise parameters (1 per instrument) and 2 RV baseline offset parameters (1 per instrument), for a total of 25 parameters.

We used a uniform prior for the RV semi-amplitude for each planet. However, we conducted a trial simulation to compare a uniform versus log uniform prior for RV semi-amplitude and found no discernible difference in our results (all parameters agreed to within  $1\sigma$ ).

# 4.6. Parameter estimation

We conducted parameter estimation of our model with the observed data using the Bayesian inference tool MultiNest (Feroz et al. 2009, 2013). We set MultiNest to constant efficiency mode, importance nested sampling mode, and multimodal mode. We used a sampling efficiency of 0.01, 1000 live points, and an evidence tolerance of 0.1. Constant efficiency is typically off, but we turned it on since it allows for better exploration of parameter space in higher-dimensional models such as our own. Further, sampling efficiency is usually set to 0.8 and the number of live points is usually set to 400. Decreasing sampling efficiency and increasing the number of live points leads to more complete coverage of parameter space, at the cost of a typically longer simulation convergence time. Finally, the evidence tolerance is usually set to 0.8; reducing the evidence tolerance causes the simulation to run longer but increases confidence that the simulation has fully converged. In other words, the standard MultiNest settings would likely lead to reliable results, but our choice of settings increases the trustworthiness of our parameter estimation and model evidence

# 4.7. Model Evidence Comparison

Table 3
K2-136 transit and planetary parameters

Parameter	Unit	This Paper	Priors
Planet b	1	7.07505   0.00050	II-: f/7 octoo 7 octoo
Period $P_b$	day	$7.97525 \pm 0.00073$	Unif(7.96529, 7.98529)
Time of transit $t_{0,b}$	BJD-2450000	$8679.083_{-0.074}^{+0.075} \\ 0.01370_{-0.00036}^{+0.00041}$	Unif(8678.58762, 8679.58762)
Planet-star radius ratio $R_b/R_*$	-	$0.01370^{+0.00041}_{-0.00036}$	Jeffreys(0.001, 0.1)
Radius $R_b$	$\mathrm{R}_{\oplus}$	$1.014^{+0.050}_{-0.049}$	
Transit duration $T_{14,b}$	hr	$2.67^{+0.086}_{-0.084}$	Unif(0, 7.2)
Impact parameter $b_b$	-	$0.22^{+0.15}_{-0.14}$	Unif(0, 1)
Semi-major axis $a_b$	$\mathrm{AU}$	$0.0707 \pm 0.0012$	
Mean density $\rho_b$	$ ho_\oplus$	$< 2.8^{\rm b}, < 4.4^{\rm c}$	•••
Mean density $\rho_b$	${ m g~cm^{-3}}$	$< 16^{\rm b}, < 24^{\rm c}$	
Insolation flux $S_b$	$\mathrm{S}_{\oplus}$	$33.5_{-1.5}^{+1.6}$	•••
Equilibrium temperature $T_{eq,b}$ (albedo = 0.3)	K	610	
Equilibrium temperature $T_{eq,b}$ (albedo = 0.5)	K	560	
Planet c			
Period $P_c$	day	$17.30723^{+0.00019}_{-0.00020}$ $8678.0792^{+0.0088}_{-0.0096}$	Unif(17.30514, 17.30914)
Time of transit $t_{0,c}$	BJD-2450000	$8678.0792_{-0.0096}^{+0.0088}$	Unif(8677.0747, 8679.0747) <sup>a</sup>
Planet-star radius ratio $R_c/R_*$	-	$0.04064^{+0.00068}_{-0.00071}$	Jeffreys(0.001, 0.1)
Radius $R_c$	$R_{\oplus}$	$3.00 \pm 0.13$	
Transit duration $T_{14,c}$	hr	$3.449^{+0.039}_{-0.031}$	Unif(0, 7.2)
Impact parameter $b_c$	-	$0.31^{+0.11}_{-0.14}$	Unif(0, 1)
Semi-major axis $a_c$	$\mathrm{AU}$	$0.1185^{+0.0020}_{-0.0021}$	<b>(</b> )
Mean density $\rho_c$	$\rho_{\oplus}$	$0.67^{+0.12}_{-0.10}$	
•	$g \text{ cm}^{-3}$	$3.69^{+0.67}_{-0.56}$	
Mean density $\rho_c$			
Insolation flux $S_c$	$S_{\oplus}$	$11.91^{+0.57}_{-0.53}$	•••
Equilibrium temperature $T_{eq,c}$ (albedo = 0.3) Equilibrium temperature $T_{eq,c}$ (albedo = 0.5)	K K	$470 \\ 440$	
Planet d			
Period $P_d$	day	$25.5750_{-0.0021}^{+0.0022} \\ 8675.936_{-0.068}^{+0.072}$	Unif(25.5551,25.5951)
Time of transit $t_{0,d}$	BJD-2450000	$8675.936^{+0.072}$	Unif(8675.4401, 8676.4401) <sup>a</sup>
Planet-star radius ratio $R_d/R_*$	_	$0.02110 \pm 0.00057$	Jeffreys(0.001, 0.1)
_,	D .	$1.565^{+0.077}_{-0.076}$	* ( , , ,
Radius $R_d$	$R_{\oplus}$	$3.04^{+0.10}_{-0.00}$	
Transit duration $T_{14,d}$	hr	-0.03	Unif(0, 7.2)
Impact parameter $b_d$	-	$0.677^{+0.042}_{-0.049}$	Unif(0, 1)
Semi-major axis $a_d$	$\mathrm{AU}$	$0.1538^{+0.0026}_{-0.0027}$	•••
Mean density $\rho_d$	$ ho_\oplus$	$< 0.35^{\rm b}, < 0.79^{\rm c}$	•••
Mean density $\rho_d$	$\mathrm{g~cm^{-3}}$	$< 1.9^{\rm b}, < 4.3^{\rm c}$	
Insolation flux $S_d$	$\mathrm{S}_{\oplus}$	$7.07_{-0.32}^{-0.34}$	
Equilibrium temperature $T_{eq,d}$ (albedo = 0.3)	K	420	
Equilibrium temperature $T_{eq,d}$ (albedo = 0.5)	K	380	
System parameters		10.22	
$Kepler/K2$ quadratic limb-darkening parameter $q_{1,Kepler}$	-	$0.38^{+0.22}_{-0.13}$	Unif(0, 1)
$Kepler/K2$ quadratic limb-darkening parameter $q_{2,Kepler}$	-	$0.38_{-0.13}^{+0.13} \\ 0.56_{-0.18}^{+0.24}$	Unif(0, 1)
K2 Campaign 13 normalized baseline offset	ppm	$0.7^{+2.9}_{-3.0}$	Unif(-1000, 1000)
K2 Campaign 13 photometric white noise amplitude	ppm	$53.9 \pm 1.8$	ModJeffreys(1, 1000, 0)

 $<sup>^{\</sup>mathrm{a}}t_{0}$  centered between K2 and TESS photometry, so ephemeris drift is incorporated into  $t_{0}$  and P.

One of the strengths of MultiNest is that it automatically calculates the Bayesian evidence of the selected model, making model comparison very easy. We compared the model evidences of eight different models (RV only, no photometry), based on all possible combinations of planets b, c, and d. The results of our model comparisons are listed in Table 5. We find that the most preferred model is the one that contains only planet c, and not planets b or d. In fact, using the Bayes factor interpretation of Kass & Raftery (1995), we find that almost every other combinations of planets can be decisively ruled out (i.e. the Bayes factor of the planet c model to any other model is > 100). The only excep-

tions are the model with planets b and c and the model with planets c and d, which are only strongly disfavored. This tells us that neither K2-136b nor K2-136d are unambiguously detected, so including either in the model quickly worsens the model evidence. However, it is notable that the model with planets b and c is better than the model with planets c and d, and is nearly in the more likely "Disfavored" category rather than "Strongly disfavored". This makes sense, as K2-136b (unlike K2-136d) has a non-zero peak in its semi-amplitude posterior distribution (see Fig. 5). In fact, although only upper limits are reported for the mass of K2-136b in Table 4, the median mass is actually non-zero at the  $2.0\sigma$  level ( $M_b$  =

K2-136c13

Table 4 K2-136 RV model parameters

Parameter	Unit	This Paper	Priors
Planet b			
Period $P_b$	day	$7.97520 \pm 0.00079$	$Normal(7.97529, 0.00080)^a$
Time of transit $t_{0,b}$	BJD-2450000	$7817.7563^{+0.0046}_{-0.0048}$	$Normal(7817.7563, 0.0048)^a$
Semi-amplitude $K_b$	${ m m~s^{-1}}$	$< 1.2^{\rm b}, < 1.7^{\rm c}$	Unif(0.001, 20)
Eccentricity $e_b$	-	$0.14^{+0.12}_{-0.11} \ (< 0.21^{\rm b}, < 0.32^{\rm c})$	d, e
Argument of periastron $\omega_b$	degrees	$189_{-132}^{+82}$	d, e
Mass $M_b$	$\mathrm{M}_{\oplus}$	$< 2.9^{\rm b}, < 4.3^{\rm c}$	
Planet c			
Period $P_c$	day	$17.30713 \pm 0.00027$	$Normal(17.30714, 0.00027)^a$
Time of transit $t_{0,c}$	BJD-2450000	$7812.71770^{+0.00086}_{-0.00085}$	$Normal(7812.71770, 0.00089)^a$
Semi-amplitude $K_c$	${ m m~s^{-1}}$	$5.49^{+0.54}_{-0.52}$	Unif(0.001, 20)
Eccentricity $e_c$	-	$0.047^{+0.062}_{-0.034} \ (< 0.074^{\rm b}, < 0.16^{\rm c})$	d
Argument of periastron $\omega_c$	degrees	$124 \pm 99$	d
Mass $M_c$	${ m M}_{\oplus}$	$18.1^{+1.9}_{-1.8}$	
Planet d			
Period $P_d$	day	$25.5750^{+0.0024}_{-0.0023}$	$Normal(25.5751, 0.0024)^a$
Time of transit $t_{0,d}$	BJD-2450000	$7780.8117 \pm 0.0065$	$Normal(7780.8116, 0.0065)^a$
Semi-amplitude $K_d$	${ m m~s^{-1}}$	$< 0.36^{\rm b}, < 0.78^{\rm c}$	Unif $(0.001, 20)$
Eccentricity $e_d$	-	$0.071^{+0.063}_{-0.049} (< 0.10^{\rm b}, < 0.16^{\rm c})$	d, e
Argument of periastron $\omega_d$	degrees	$280^{+130}_{-110}$	d, e
Mass $M_d$	${ m M}_{\oplus}$	$< 1.3^{\rm b}, < 3.0^{\rm c}$	
System and GP parameters	1 1	0.4.1.0.5	TT 10/ 00F 00F)
RV slope	${\rm m}\ {\rm s}^{-1}\ {\rm yr}^{-1}$	$0.1 \pm 2.5$	Unif(-365, 365)
HARPS-N RV white noise amplitude	m s <sup>-1</sup>	$0.83 \pm 0.52$	Unif(0, 20)
ESPRESSO RV white noise amplitude	$\mathrm{m}\ \mathrm{s}^{-1}$	$1.57^{+0.73}_{-0.62}$	Unif(0, 20)
HARPS-N RV offset amplitude	$\mathrm{m}~\mathrm{s}^{-1}$	$39503.7_{-1.9}^{+2.1}$	Unif(39450, 39550)
ESPRESSO RV offset amplitude	$\mathrm{m}~\mathrm{s}^{-1}$	$39494.7^{+3.5}_{-3.6}$	Unif(39450, 39550)
GP RV convective blueshift amplitude $V_c$	${ m m~s^{-1}}$	$3.5^{+2.2}_{-1.2}$	Unif(0, 100)
GP RV rotation modulation amplitude $V_r$	${ m m~s^{-1}}$	$22.0_{-8.0}^{-112.9}$	Unif(0, 100)
GP stellar rotation period $P_*$	day	$13.37^{+0.13}_{-0.17}$	Unif(1, 20)
GP inverse harmonic complexity $\lambda_p$		$0.75^{+0.23}_{-0.16}$	Unif(0.1, 3)
GP evolution time-scale $\lambda_e$	day	$48^{+19}_{-11}$	Unif(1, 200)

<sup>&</sup>lt;sup>a</sup>Mann et al. (2018)

Table 5 Model Evidence Comparisons for K2-136 Planet Configurations

Planets in model	$\Delta \log_{10}(\text{evidence})$	Interpretation
c	0	-
b,c	-1.10	Strongly disfavored
$_{\mathrm{c,d}}$	-2.06	Strongly disfavored
b,c,d	-3.23	Excluded
-	-5.54	Excluded
d	-7.00	Excluded
b	-7.78	Excluded
b,d	-9.17	Excluded

# $2.4 \pm 1.2 \text{ M}_{\oplus}$ ).

Our results tell us that we can be confident that K2-136c has been detected in our observations. In contrast, the RV signals of K2-136b and K2-136d fall below the threshold of detection, at least given the quantity and quality of our specific data set. Continued radial velocity monitoring, particularly with high precision instruments and facilities may be able to measure their masses, especially K2-136b (which appears to already be near the threshold of detection with our current data set).

Although the model with only K2-136c is the most favored, we still use a model with all three planets as our canonical model for parameter estimation for three reasons. First, we already know from transit photometry that planets b and d exist. Accordingly, the goal of the model comparison exercise described above is not to question the existence of these planets but to examine whether the RV signals from each planet can be detected

 $<sup>^{\</sup>rm b}68\%$  confidence limit

 $<sup>^{\</sup>rm c}95\%$  confidence limit

 $<sup>^{\</sup>rm d}$ Unif(-1, 1) on  $\sqrt{e}\sin\omega$  and  $\sqrt{e}\cos\omega$ . See Eastman et al. (2013).  $^{\rm e}$ K2-136b and K2-136d had additional eccentricity prior upper limits of 0.35 and 0.37, respectively; see Section 4.5.

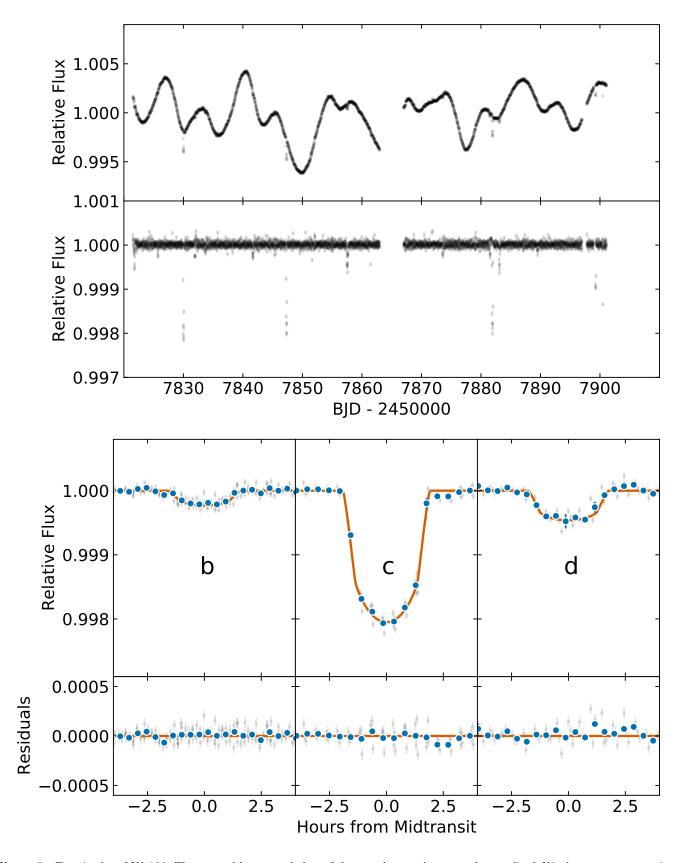


Figure 3. Transit plot of K2-136. The top and bottom subplots of the top plot are the raw and normalized K2 photometry versus time from Campaign 13, respectively. In the top subplots of the bottom plot are the phase-folded light curves and transit model fits for K2-136b, c, and d. The gray points are the raw data. The best-fit transit model is the orange line and binning is represented by the blue points. The bottom subplots of the bottom plot are the residuals after the best-fit model has been subtracted.

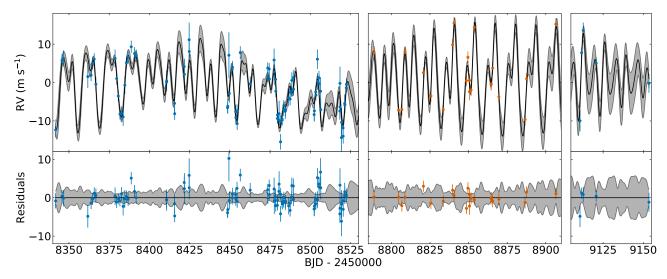


Figure 4. K2-136 observations and model fits for RVs (and fit residuals). In each panel, the blue points (HARPS-N) or orange points (ESPRESSO) are the observations while the black line and gray region are the model fit and  $1\sigma$  confidence interval, respectively. RVs have been mean-subtracted (corresponding to their respective instrument) and planet-induced reflex motion has been subtracted as well. RV errors have been inflated from their original values by adding the model-estimated RV jitter term in quadrature. Note the two time gaps between the first 88 HARPS-N observations, the 22 ESPRESSO observations, and the final 5 HARPS-N observations.

in our data set. By adopting the three-planet model, we incorporate the uncertainties introduced by the unknown masses and eccentricities of planets b and d. Second, using the three-planet model allows us to determine upper limits for the masses of planets b and d, which is useful for constraining planet compositions and providing guidance for any future attempts to constrain the mass of either planet. Third, both models agree very closely: all parameters are consistent at  $1\sigma$  or less, and all uncertainties on parameters are similar in scale. For the RV semi-amplitude of K2-136c, our key parameter of interest, our canonical model returned  $K_c = 5.49^{+0.54}_{-0.52}$  m s<sup>-1</sup> while the one-planet model returned  $K_c = 5.17^{+0.56}_{-0.51}$  m s<sup>-1</sup>.

## 4.8. Model Reliability Tests

In order to rigorously assess the accuracy of our results, we conducted tests to analyze different components of our model. Specifically, we removed the GP portion of the model, and we also injected and recovered synthetic planets into the system to compare input and output RV semi-amplitudes.

For our test models we chose not to include planets b and d, as well as photometry, and we then compared against the model with only K2-136c (hereafter referred to as the "one-planet reference model") rather than the three-planet model; this is despite already selecting the three-planet model as the canonical model to report our results (see Section 4.7). This was done for a few reasons. First, the one-planet model is the preferred model according to the Bayesian evidences, so it is a reasonable point of comparison. Second, as stated earlier, the one-planet reference model and the three-planet model agree very closely. Therefore, any test model parameters found to be highly consistent with the one-planet reference model results will also be highly consistent with the three-planet model results. Third, as a practical matter, including only K2-136c in our test models significantly

reduced computational complexity, allowing us to test a wider variety of models.

## 4.8.1. No GP

GPs are very versatile and can fit highly variable and correlated signals. Therefore, it is reasonable to ask whether a GP may, in the process of modeling stellar activity, "steal" part of the RV signal from a planet due to overfitting of the data. In order to address these concerns, we ran a model without a GP, and no alternative method to handle stellar activity. We found the resulting parameters were broadly consistent. The noise parameters for each data type in the no-GP model were notably larger, but that is to be expected given no mitigation of the stellar activity. All other parameters agreed with the one-planet reference model parameters to within  $1\sigma$ ; for the RV semi-amplitude of K2-136c, we determined a value of  $K_c = 5.92^{+0.89}_{-0.91}$  m s<sup>-1</sup> (compared to  $K_c = 5.17^{+0.56}_{-0.51}$  m s<sup>-1</sup> for the one-planet reference model). Finally, it is greatly and model). Finally, it is worth noting we also found that  $\Delta \log_{10}(\text{evidence}) = -18.1 \text{ compared to the one-planet}$ reference model, decisively ruling out the no-GP model (Kass & Raftery 1995). In other words, a GP accounts for the stellar activity satisfactorily, whereas ignoring stellar activity is clearly insufficient.

## 4.8.2. Synthetic Planet Injections

We also conducted planet injection tests to determine how robustly we could recover the injected signals. Accurate recovery of such signals builds confidence in the accuracy of the RV signal recovered for K2-136c as well as the upper limits placed on K2-136b and K2-136d.

We ran four separate tests in which we injected a 5.5 m s<sup>-1</sup> RV signal of a planet on a circular orbit with a period of 4, 12, 20, and 28 days. 5.5 m s<sup>-1</sup> was chosen because it is approximately the same semi-amplitude as the signal induced by K2-136c, allowing us to directly test our confidence in the recovered RV signal of K2-

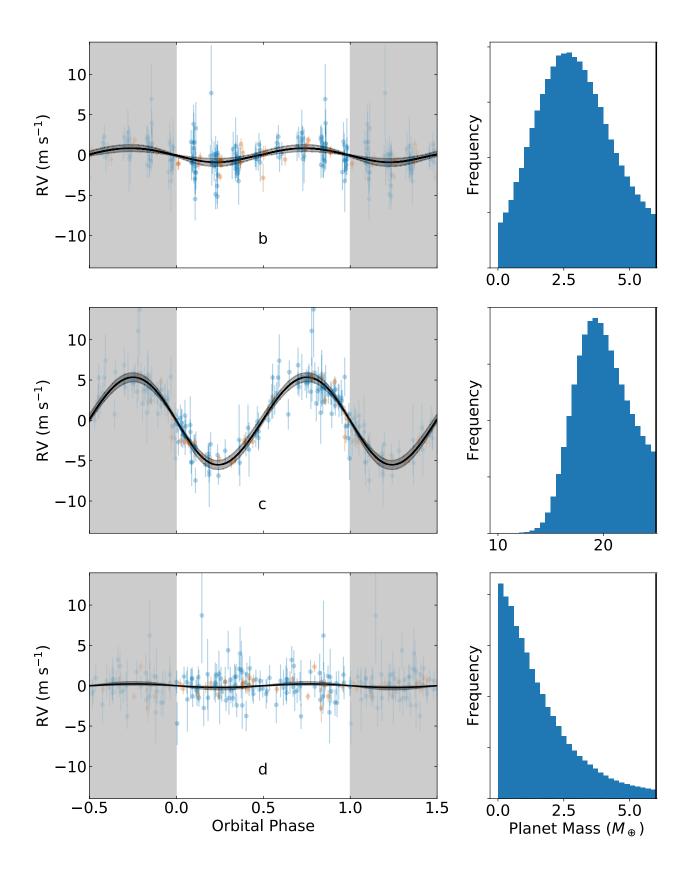


Figure 5. Left: Phased RV plots for all three K2-136 planets. For each subplot, we used our best fit model parameters to remove stellar activity and the presence of the other two planets. In each subplot, blue data points (HARPS-N) and orange data points (ESPRESSO) are unbinned RV observations. The black line is the median fit and the gray region around that line is the  $1\sigma$  confidence interval. Right: Posterior mass distribution plots for all three K2-136 planets. It is visually apparent that while there is a strong mass detection for K2-136c  $(R_p = 3.00 \pm 0.13 \text{ R}_{\oplus})$ , there is at best only a marginal detection for K2-136b  $(R_p = 1.014 \pm 0.050 \text{ R}_{\oplus})$  and no evidence of a detection for K2-136d  $(R_p = 1.565 \pm 0.077 \text{ R}_{\oplus})$ . Therefore, therefore we report only place upper limits on the masses of K2-136b and K2-136d (see Table 4).

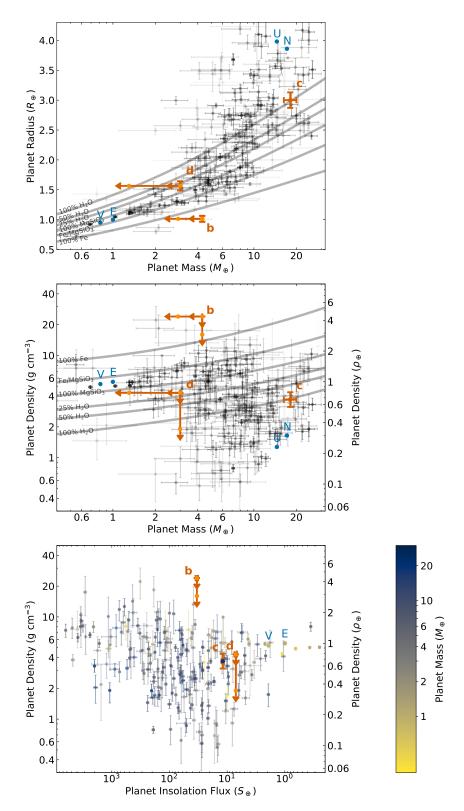


Figure 6. Top: mass-radius diagram of transiting planets with fractional mass and radius uncertainties less than 50%. K2-136b, c, and d are plotted in dark orange, with mass uncertainties on K2-136b and d as 68% and 95% upper limits denoted in light orange. Data collected from the NASA Exoplanet Archive (accessed 2023 Mar 22; NASA Exoplanet Science Institute 2020). Venus, Earth, Uranus, and Neptune are also labeled and plotted in blue for reference. Except for the K2-136 system, planets with larger fractional mass and radius uncertainties are fainter. Gray lines correspond to planetary compositions (from top to bottom) of 100% H<sub>2</sub>O, 50% H<sub>2</sub>O, 25% H<sub>2</sub>O, 100% MgSiO<sub>3</sub>, 50% MgSiO<sub>3</sub> + 50% Fe, and 100% Fe, respectively (Zeng & Sasselov 2013; Zeng et al. 2016). Kepler-136c lies closest to the 100% H<sub>2</sub>O composition line, and is similar in mass to Uranus and Neptune although smaller and much more dense. Middle: the same sample plotted in mass versus planet density, with the same solar system references and composition lines (order inverted from top panel). Bottom: the same sample plotted in planet insolation flux versus planet density, with the color of all data points corresponding to planet mass (except K2-136b and d, which only have mass upper limits and thus are plotted in light orange).

MAYO ET AL.

136c specifically. Our set of orbital periods was selected in order to 1) span the range of known periodic signals in the system (the orbital period of the three known planets and the stellar rotation period), 2) avoid close proximity to those signals (none are within 1.5 days of the injected signals), and 3) be equally spaced in order to uniformly test the encompassed period range.

All four of the recovered signals agree with the injected signal of 5.5 m s<sup>-1</sup> to within  $1\sigma$ . In all four tests, the recovered signal of K2-136c also agrees with our one-planet reference model ( $K_c = 5.28 \pm 0.56$  m s<sup>-1</sup>) within  $1\sigma$ , lending further confidence to our results.

# 4.9. High-Energy Observations 4.9.1. HST NUV observations


To compare the UV quiescent activity of K2-136 with other K stars Hyades members, we measured the surface flux of the Mg II h (2796.35 Å) and k (2808.53 Å) lines. The Mg II lines are the strongest emission lines in the NUV and correlate strongly with the chromospheric activity of the star. For accurate emission measurements, we subtracted the NUV continuum by fitting the data outside of the Mg II integration region using the astropy module specutils. We then integrated over 2792.0-2807.0 Å to measure the Mg II emission flux. To convert from observed flux to surface flux, we estimated the radii of the stars using the relationships between age, effective temperature, and radius given by Baraffe et al. (2015), except for K2-136, where we use the radius reported in this work.

Figure 7 shows the Mg II surface flux as a function of the rotation period for K2-136 and 13 other observed K star members of the Hyades from GO-15091. K2-136 has a surface Mg II flux of  $(8.32 \pm 0.17) \times 10^5$  erg s<sup>-1</sup> cm<sup>-2</sup>, whereas the median of the sample is  $(9.66 \pm 0.24) \times 10^5$  erg s<sup>-1</sup> cm<sup>-2</sup>.

Additionally, Richey-Yowell et al. (2019) measured the NUV flux densities of 97 K stars in the Hyades using archival data from the *Galaxy Evolution Explorer* (*GALEX*; Martin et al. 2005). The median NUV flux density of their sample of Hyades stars at a normalized distance of 10 pc was  $1.89 \times 10^3 \mu \text{Jy}$ . We measure a *GALEX* NUV magnitude for K2-136 of 19.51 mag, which corresponds to a flux density at 10 pc of  $1.52 \times 10^3 \mu \text{Jy}$ , well within the interquartiles of the total sample from Richey-Yowell et al. (2019).

## 4.9.2. X-ray observations

We detected a total of 800 EPIC counts for K2-136 in the XMM observation and can therefore extract an X-ray spectrum for the star. We used a one-temperature APEC model to fit the spectrum, which is appropriate for representing the hot plasma in stellar coronae. We combined this model with the ISM absorption model tbabs using photoelectric cross-section from Balucinska-Church & McCammon (1992) to account for the neutral hydrogen column density  $N_{\rm H}$ . We set  $N_{\rm H}$  to  $5.5 \times 10^{18}$  cm<sup>-2</sup>, derived using E(B-V)=0.001 for Hyades (Taylor 2006),  $R_V=3.1$ , and the relation  $N_{\rm H}[{\rm cm}^{-2}/A_v]=1.79\times 10^{21}$  (Predehl & Schmitt 1995); allowing  $N_{\rm H}$  to float did not improve the fit. The spectra for each of the three XMM cameras are shown in Figure 8 and the best-fit parame-

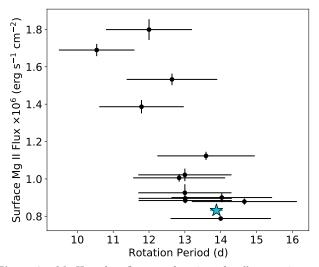

**Figure 7.** Mg II surface flux as a function of stellar rotation period for K star Hyades members. The blue star represents K2-136, and the black points are the 13 other K star Hyades observed in a broader HST program (GO-15091, PI: Agüeros). The rotation periods are from Douglas et al. (2019) and have assumed errors of 10%, except for K2-136, which we determined to be  $13.88^{+0.17}_{-0.18}$  d in this work. K2-136 does not show any distinct chromospheric activity or unique rotation period compared to the rest of the sample.

ters, which are obtained from a simultaneous fit to the three, are provided in Table 6.

Using the total EPIC energy flux from the spectral best fit, we obtained an X-ray luminosity  $L_{\rm X}=(1.26\pm0.19)\times10^{28}~{\rm erg~s^{-1}}$  and  $L_{\rm X}/L_{*}=(1.97\pm0.30)\times10^{-5}$  (0.1–2.4 keV energy range). These values are within  $1\sigma$  of those found by Fernandez Fernandez & Wheatley (2021) using the same XMM observation<sup>4</sup>. For the sample of 89 K dwarfs with X-ray detections in the Hyades, the median values for  $L_{\rm X}$  and  $L_{\rm X}/L_{*}$  are  $4.5^{+7.9}_{-3.3}\times10^{28}$  erg s<sup>-1</sup> and  $4.0^{+20.8}_{-1.6}\times10^{-5}$ , respectively (Núñez et al. in prep.). K2-136, therefore, appears somewhat less luminous in X-rays than most of its coeval K dwarf brethren. A narrower comparison, against late-K (K5 and later) dwarf Hyads, shows that the  $L_{\rm X}$  and  $L_{\rm X}/L_{*}$  values for K2-136 are within one standard deviation of the median for that cohort.

In addition to X-ray luminosity, we also estimated extreme ultraviolet (EUV) luminosity using stellar age and Equation 4 from Sanz-Forcada et al. (2011) and found  $L_{\rm EUV}=(22.6^{+7.8}_{-5.7})\times 10^{28}~{\rm erg~s^{-1}}$ . Combining  $L_{\rm X}$  and  $L_{\rm EUV}$  and using the semi-major axis of K2-136c, we are able to estimate the X-ray and UV flux incident on K2-136c to be  $F_{\rm XUV}=(6.0^{+2.0}_{-1.4})\times 10^3~{\rm erg~s^{-1}~cm^{-2}}$ . Then, using this incident flux value (along with  $\rm M_c$  and  $\rm R_c)$  we estimate an atmospheric mass loss rate with Equation 1 from Foster et al. (2022). This yields a current atmospheric mass loss rate for K2-136c of  $\dot{M}_{\rm c}=(3.4^{+1.3}_{-0.9})\times 10^9~{\rm g~s^{-1}}=(17.8^{+6.7}_{-5.0})\times 10^{-3}~{\rm M}_{\oplus}~{\rm Gyr^{-1}}$ . This rate is based on current values, so the mass loss rate in the past or future may differ. At this current rate, with a  $\rm H_2$ -He envelope mass fraction of  $\sim 5\%$ , it would take  $\rm 51^{+23}_{-16}~{\rm Gyr}$ 

<sup>&</sup>lt;sup>4</sup> These authors performed spectral fitting (using a three-temperature APEC model) only to the EPIC pn detection to derive the X-ray energy flux for K2-136.

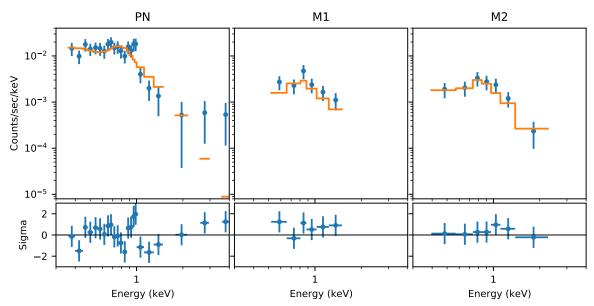


Figure 8. X-ray spectra of K2-136 from the XMM pn (left panel), MOS1 (center), and MOS2 (right) EPIC cameras. X-ray counts are binned by 20 in the pn camera, and 15 in the MOS cameras. The orange lines are the best fits using a one-temperature APEC model and assuming a fixed neutral hydrogen column density of  $5.5 \times 10^{18}$  cm<sup>-2</sup>, typical for Hyads (see Sec. 4.9.2). The residuals of each fit are shown in the bottom panels. The best-fit parameters are presented in Table 6.

to fully evaporate the atmosphere. Even the 95% lower limit evaporation time is still 28 Gyr, longer than the age of the universe. In other words, in  $\sim 4$  Gyr, when the K2-136 system is as old as the Solar System currently is, we expect K2-136c will have likely only lost 5-10% of its current atmosphere.

We also calculated the Rossby number  $R_o$  of K2-136, which is defined as the star's rotation period  $P_*$  divided by the convective turnover time  $\tau$ . We used the  $(V-K_s)$ -log  $\tau$  empirical relation in Wright et al. (2018) (their equation 5) to obtain  $\tau=22.3$  d for K2-136. Using our measured  $P_*$  value (see Sec. 3.1) gives  $R_o=0.6$ . This  $R_o$  puts K2-136 well within the X-ray unsaturated regime, in which the level of magnetic activity decays follows a power slope as a function of  $R_o$  (see figure 3 in Wright et al. 2018). For the sample of 51 K dwarf rotators with X-ray detection in the Hyades, the median  $R_o=0.46^{+0.06}_{-0.08}$  (Núñez et al, in prep.), which suggests that the lower levels of X-ray emission from K2-136 relative to its fellow Hyades K dwarfs can be explained by its slower rotation rate.

In conclusion, K2-136 does not appear unusually active in either the NUV or the X-ray relative to its fellow Hyades K dwarfs.

## 4.10. Considering the Nearby Stellar Companion

As discussed in Section 3.2, prior observations of this system revealed a likely bound M7/8V companion with a projected separation of approximately 40 AU. The presence of a nearby stellar companion can easily cause a trend in RV observations. We wanted to estimate the range of possible trend amplitudes for our system using some reasonable assumptions. Using the distance of  $58.752^{+0.061}_{-0.072}$  pc from Bailer-Jones et al. (2021) and the projected angular separation of  $0.730 \pm 0.030$ " from adding in quadrature the R.A. and Dec separation components in Ciardi et al. (2018), we found a projected separation of  $42.9 \pm 1.7$  AU. We considered the possibil-

Table 6
X-ray Spectral Fit Parameters of K2-136

<sup>&</sup>lt;sup>a</sup>All flux values are in the 0.1–2.4 keV energy range.

ity of additional radial separation by folding in a uniform distribution on radial separation between 0 and twice the median projected separation to estimate an overall separation (this broad range was chosen to include radial separations of approximately the same scale as the projected separation). As an approximation, we treat this overall separation as the semi-major axis.

Next, the stellar companion was reported in Ciardi et al. (2018) to have a spectral type consistent with M7/8 (we were unable to find uncertainties associated with this result, but nearby spectral types were never mentioned). Taking a conservative approach, we assumed a stellar companion mass between 1  $\rm M_{Jup}$  (for a low-mass brown dwarf) and 0.2  $\rm M_{\odot}$  (for a mid to late M dwarf).

Then, we combined our separation distribution and stellar mass distributions (primary and companion) via Kepler's Third Law to get a broad orbital period estimate of  $520^{+320}_{-180}$  years. Including a wide range of eccentricities (Unif(0,0.9)), we estimated an RV semi-amplitude of  $490^{+340}_{-320}$  m s<sup>-1</sup>. On the timescale of our observations, this centuries-long sinusoidal signal would manifest as a linear trend, with a maximum (absolute) slope of  $5.3^{+7.5}_{-3.6}$ 

<sup>&</sup>lt;sup>b</sup>The error-weighted average of the pn and MOS cameras.

m s<sup>-1</sup> yr<sup>-1</sup>. This is a very rough estimate with many assumptions, but it serves to demonstrate that a drift of only a few m s<sup>-1</sup> each year or less is very reasonable. Indeed, from our model of the RV data we found an RV trend of  $0.1\pm2.5$  m s<sup>-1</sup> yr<sup>-1</sup>, highly consistent with both a zero trend as well as our estimate calculated here.

#### 5. RESULTS AND DISCUSSION

The results of our stellar and planet analyses are listed in Tables 1, 4, and 3. Phase plots of all three planets can be seen in Fig. 5. After conducting our analysis and tests, we find that K2-136c has a mass of  $18.1^{+1.9}_{-1.8}$  M $_{\oplus}$  and a radius of  $3.00\pm0.13$  R $_{\oplus}$ . This radius is consistent with and slightly larger than the value estimated in M18  $(2.91^{+0.11}_{-0.10}$  R $_{\oplus})$ . This is because we find a stellar radius value slightly larger than M18 (by about 3%).

Using planet mass and radius we find K2-136c has a density of  $3.69^{+0.67}_{-0.56}$  g cm<sup>-3</sup> (or  $0.67^{+0.12}_{-0.10}$   $\rho_{\oplus}$ ). For comparison, Neptune<sup>2</sup> is roughly similar in mass (17.15  $M_{\oplus}$ ) but larger in radius (3.883  $R_{\oplus}$ ); as a result, K2-136c is more than twice as dense as Neptune ( $2.25^{+0.41}_{-0.34}$   $\rho_{\oplus}$ ). Similarly, Uranus<sup>3</sup> is slightly less massive (14.54  $M_{\oplus}$ ) but still larger in radius (4.007  $R_{\oplus}$ ); thus, K2-136c is nearly three times as dense as Uranus ( $2.90^{+0.52}_{-0.44}$   $\rho_{\oplus}$ ). This is visually apparent in Fig. 6, which shows K2-136c almost perfectly on the 100%  $H_2O$  composition line. It is important to remember that mass and radius alone do not fully constrain a planet's composition. Although K2-136c may have a density similar to that of a large ball of water (an unrealistic reference composition), it is also consistent with a gaseous sub-Neptune with a massive core or metal-rich atmosphere.

Unfortunately, it is very difficult to determine compositional properties of a planet without atmospheric characterization, especially sub-Neptunes (since there are no analogs in our own Solar System). On the one hand, sub-Neptunes may include ocean worlds with H<sub>2</sub>O abundance fractions not seen in our Solar System (Mousis et al. 2020). And indeed, water vapor has already likely been detected in the atmosphere of the sub-Neptune exoplanet K2-18b (Benneke et al. 2019b). On the other hand, sub-Neptunes like K2-136c may instead be composed of a rocky, Earth-like core composition, very little water, and an atmosphere close to solar metallicity and thus primarily hydrogen and helium (Van Eylen et al. 2018; Benneke et al. 2019a).

As a valuable point of comparison, there are three confirmed planets that share a similar mass and radius to K2-136c to within 10%: Kepler-276c, Kepler-276d (Xie 2014), and TOI-824b (Burt et al. 2020). The masses of the planets in the Kepler-276 system were measured via transit timing variations (TTVs) in a TTV catalog paper. Unfortunately, because they were characterized alongside so many other systems, there is no discussion regarding the formation or composition of those two specific planets. TOI-824b, however, was characterized in a standalone paper that investigated the nature of the planet thoroughly. Unlike K2-136c, TOI-824b is near

the hot-Neptune desert (Mazeh et al. 2016) with a very short orbital period (1.393 d). Despite its proximity to its host star, TOI-824b still retains a  $\rm H_2\text{-He}$  atmosphere, which the authors estimate has a mass fraction of  $\geq 2.8\%$ . They hypothesize that the larger than average mass of the planet (compared to planets of a similar radius) helps the planet retain its atmosphere. K2-136c, with a similar mass and radius and a lower insolation flux, would therefore be able to retain a  $\rm H_2\text{-He}$  atmosphere even more easily.

We can go further and form a picture of a reasonable composition for K2-136c. We may assume the planet has a rocky core surrounded by a gaseous  $H_2$ -He envelope. Going a step further, we may also assume the rocky core is similar to that of Earth, namely a core-mass fraction (CMF) of 0.325, i.e. a rock-iron composition of 32.5% Fe and 67.5% MgSiO<sub>3</sub> (Seager et al. 2007). Following the theoretical models of Howe et al. (2014), we find that with an Earth-like rocky core and a  $H_2$ -He envelope, the measured mass and radius of K2-136c are most consistent with a  $H_2$ -He mass fraction of  $\sim 5\%$ .

With this rough envelope mass fraction estimate and the measured mass and radius of K2-136c, we wanted to investigate the potential for past or ongoing atmospheric mass loss. After consulting the theoretical models presented in Lopez et al. (2012), Lopez & Fortney (2013), Lopez & Fortney (2014), and Jin et al. (2014), we concluded that if there is any historical or contemporary mass loss for K2-136c, it is minimal: likely somewhere between 0-10% loss of the H<sub>2</sub>-He envelope across the entire lifespan of the planet.

As suggested in Mann et al. (2016), young planets may be puffier than older planets due to an early-age atmospheric mass loss phase. And yet, K2-136c is not particularly puffy, in fact being notably denser than Uranus or Neptune. However, this planet may indeed have an extended atmosphere but also a lower atmospheric mass fraction than Uranus, Neptune, and other lower-density planets. In other words, as this system ages, the atmosphere of K2-136c may settle to some extent, reducing the planet radius and increasing planet density. Without atmospheric characterization, further insights into the planet's composition are very limited.

Bayesian model comparison proved that we could not conclusively detect K2-136b or K2-136d in our data set (see Fig. 5). Even so, we also conduct similar analyses for K2-136b and K2-136d in order to report upper mass limits and corresponding upper density limits. With 95% confidence, K2-136b is no denser than 24 g cm<sup>-3</sup> (a largely unhelpful limit, since that would be much more dense than pure iron) and K2-136d is no denser than 4.3 g cm $^{-3}$ , corresponding to semi-amplitudes of 1.7 m s $^{-1}$ and 0.78 m s<sup>-1</sup>, respectively. Referring to Fig. 6, we can see that unlike the middle planet K2-136c, the other two planets K2-136b and K2-136d could have a wide variety of densities and compositions. K2-136d could range from a low-density gas planet to Earth composition. K2-136b has an even wider array of possible compositions and theoretically could range from very gaseous to pure iron.

The RV signals of K2-136b and K2-136d may be detectable with more data from next generation spectrographs. K2-136d would be particularly interesting, since its radius places it near the planet radius gap (Fulton

 $<sup>^2\</sup> https://nssdc.gsfc.nasa.gov/planetary/factsheet/neptunefact.html$ 

<sup>&</sup>lt;sup>3</sup> https://nssdc.gsfc.nasa.gov/planetary/factsheet/uranusfact.html

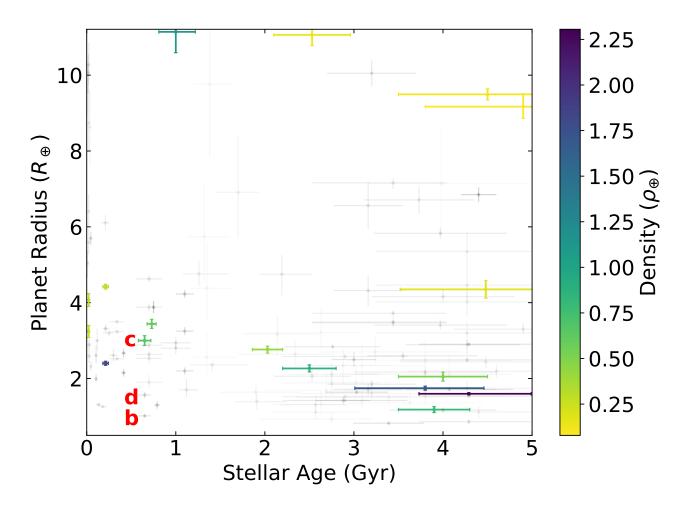


Figure 9. Age-radius diagram for all planets smaller than Jupiter, younger than 5 Gyr, and with radius and age uncertainties both smaller than 25%. Data point color corresponds to planet density for planets with mass uncertainties smaller than 25%. Data collected from the NASA Exoplanet Archive (accessed 2023 Mar 22; NASA Exoplanet Science Institute 2020). K2-136b, c, and d are labeled in red to the left of the planet symbol. There are only four planets in this figure with a stellar age younger than K2-136 and a mass measurement better than 25%: AU Mic b and c (stellar age =  $22 \pm 3$  Myr; Mamajek & Bell 2014) and Kepler-411 b and c (stellar age =  $212 \pm 3$  Myr; Sun et al. 2019). The only other plotted planet < 1 Gyr with a mass measurement is the open cluster planet K2-25b (Stefansson et al. 2020), which is slightly larger than K2-136c.

et al. 2017). As for K2-136b, the peak of the planet mass posterior distribution is already non-zero, and a marginal detection may already be noted at the  $2.0\sigma$  level ( $2.4\pm1.2$   $M_{\oplus}$ ), suggesting a firm planet mass measurement may be within reach with further observations.

To check this, we followed the mass-radius relationship laid out in Wolfgang et al. (2016) and found predicted masses for K2-136b and K2-136d to be  $1.17^{+0.79}_{-0.72}$  M $_{\oplus}$  and  $4.1^{+1.9}_{-1.8}$  M $_{\oplus}$ , respectively. These correspond to densities of  $7.7^{+3.7}_{-4.7}$  g cm $^{-3}$  (i.e.  $1.40^{+0.66}_{-0.85}$   $\rho_{\oplus}$ ) and  $8.4^{+4.1}_{-3.7}$  g cm $^{-3}$  (i.e.  $1.52^{+0.74}_{-0.66}$   $\rho_{\oplus}$ ), respectively. We note that these mass and density estimates do not make use of the upper limits determined in this paper. By folding in our stellar mass, orbital period, and eccentricity posteriors as well as the orbital inclinations determined in M18, we found the estimated masses of K2-136b and K2-136d correspond to semi-amplitudes of  $0.5\pm0.3$  m s $^{-1}$  and  $1.1\pm0.5$  m s $^{-1}$ , respectively. The current RV upper limit on K2-136b (1.7 m s $^{-1}$ ) is much larger than the estimated semi-amplitude and therefore fully consistent. As for K2-136d, we ac-

knowledge that the estimated semi-amplitude is smaller than the upper limit  $(0.80 \text{ m s}^{-1})$ , which perhaps suggests K2-136d has a density on the lower end of the range predicted from the Wolfgang et al. (2016) relationship.

There are very few young and small exoplanets that also have measured masses. As can be seen in Fig. 9, the vast majority of young exoplanets do not have a firm mass measurement. There are some young planets with both robust radius measurements and notable upper mass limits, such as the low-density planet TS Duc A b (Benatti et al. 2021), which can be of interest for follow-up study and comparison. However, according to the NASA Exoplanet Archive (accessed 2023 Mar 12; NASA Exoplanet Science Institute 2020), there are only 13 known planets, excluding K2-136c, with  $R_p < 4 R_{\oplus}$ , a host star age < 1 Gyr, and a mass measurement (not an upper limit): HD 18599b (Desidera et al. 2022), HD 73583b and c (Barragán et al. 2022); K2-25b (Stefansson et al. 2020); L 98-59b, c, and d (Demangeon et al. 2021); Kepler-411b and Kepler-411d (Sun et al. 2019), Kepler-462b (Masuda & Tamayo 2020), Kepler-289b and Kepler-

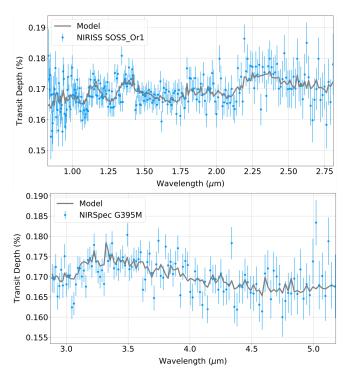


Figure 10. Simulation of JWST transmission spectra for K2-136c using JET (Fortenbach & Dressing 2020). The top and bottom panels correspond to the NIRISS SOSS-Or1 (0.81-2.81  $\mu\mathrm{m})$  instrument, and the NIRSpec G395M (2.87-5.18  $\mu\mathrm{m})$  instrument, respectively. The gray line in both panels is the modelled atmospheric spectrum assuming low metallicity (5x solar) and no clouds, while the blue data points are the simulated instrument spectra for one observed transit with NIRISS SOSS, and two observed transits with NIR-Spec G395M, including the effects of photon noise, and instrument systematics.

289d (Schmitt et al. 2014), and K2-100b (Barragán et al. 2019).

K2-136c is now the smallest exoplanet in an open cluster to have a mass measurement. It is also one of the youngest exoplanets to ever have a mass measurement. The only planets with firm age, radius, and mass measurements (< 25% uncertainties) known to be younger are AU Mic b and c (Klein et al. 2021) as well as Kepler-411b and d (Sun et al. 2019), as can be seen in Fig. 9. In general, measuring the masses of young planets like K2-136c provides an interesting window into the early childhood of planetary systems, allowing us to probe how planet masses and compositions evolve over time.

## 5.1. Atmospheric Characterization Prospects

To explore the suitability of the K2-136 system planets for atmospheric characterization, we calculated the transmission spectroscopy metric (TSM) defined in Kempton et al. (2018). K2-136c has a TSM of  $32.7^{+4.8}_{-4.1}$ , which is well below the recommended TSM of 90 for  $R_p > 1.5~{\rm R}_{\oplus}$ . Because K2-136b and K2-136d have unconstrained masses, we followed Zeng et al. (2016) and assumed an Earth-like CMF of 0.325 in order to predict planet masses of  $0.85^{+0.27}_{-0.21}~{\rm M}_{\oplus}$  and  $3.35^{+1.08}_{-0.84}~{\rm M}_{\oplus}$ , respectively. For K2-136b, this yields a TSM of  $4.20^{+0.42}_{-0.37}$ , well below the recommended TSM of 10 for  $R_p < 1.5~{\rm R}_{\oplus}$ . As for K2-136d, its radius of  $R_d = 1.565 \pm 0.077~{\rm R}_{\oplus}$  is very near  $1.5~{\rm R}_{\oplus}$ , where the TSM metric includes a scale factor that jumps dramatically, thus creating a TSM bi-

modal distribution. Thus, for  $R_d < 1.5 \text{ R}_{\oplus}$  we find a TSM of  $2.36^{+0.15}_{-0.13}$  and for  $R_d > 1.5 \text{ R}_{\oplus}$  we find a TSM of  $13.6^{+1.0}_{-1.1}$ . In their respective radius ranges, these values are both well below the recommended TSM, so K2-136d is also probably not a good target for atmospheric characterization.

We also calculated the emission spectroscopy metric (ESM) for K2-136b and K2-136d as defined in Kempton et al. (2018) (the metric applies only to "terrestrial" planets with  $R_p < 1.5~{\rm R}_{\oplus}$ , excluding K2-136c). We find K2-136b and K2-136d have ESM metrics of  $0.520^{+0.049}_{-0.047}$  and  $0.342^{+0.043}_{-0.041}$ , respectively, both below the recommended ESM of 7.5 or higher. Therefore, these planets do not appear to be particularly attractive targets for emission spectroscopy or phase curve detection.

The TSM analysis of K2-136c is not very favorable for atmospheric characterization, but we decided to conduct a more thorough transmission spectroscopy analysis. We used the JET tool (Fortenbach & Dressing 2020) to model atmospheric spectra and to simulate the performance of the JWST instruments for certain atmospheric scenarios. We opted for the broad wavelength coverage of combining NIRISS SOSS Order 1 (0.81-2.81  $\mu$ m) with NIRSpec G395M (2.87-5.18  $\mu$ m), as recommended by Batalha & Line (2017) to maximize the spectral information content. A single instrument, the NIRSpec Prism, can also cover this wavelength range, but brightness limits preclude its use here. We assumed pessimistic pre-launch instrumental noise values (Rigby et al. 2022), so a future JWST program for atmospheric characterization should outperform our conservative expectations.

The JET tool found that for an optimistic, cloudless, low-metallicity atmosphere (5x solar) we can meet a  $\Delta \text{BIC}$  detection threshold of 10 (corresponding to a  $\sim 3.6\sigma$  detection of the atmosphere compared to a flat line) with 5 free retrieval parameters (i.e., recon level) with only one transit for NIRISS SOSS and two transits for NIRSpec G395M. For a less optimistic, higher metallicity atmosphere (100x solar) with clouds at 100 mbar, we can meet the same detection threshold with two transits for NIRISS SOSS and five transits for NIR-Spec G395M.

With 10 free retrieval parameters (a more typical number), and with the optimistic atmosphere, we can meet a  $\Delta$ BIC detection threshold of 10 with only one transit for NIRISS SOSS and three transits for NIRSpec G395M. For the less optimistic atmosphere, we can meet the detection threshold with three transits for NIRISS SOSS, but we show no detection for NIRSpec G395M for up to 50 transits considered. This analysis makes the conservative assumption that the instrument noise floor is not reduced by co-adding transits.

The resulting spectra for the low metallicity, cloudless, case are shown in Fig. 10. It seems that atmospheric characterization of K2-136c may be within reach (assuming a relatively low mean molecular weight/low metallicity atmosphere, and low cloud level), but could require a more significant investment of JWST resources if the actual atmospheric properties are less favorable.

It should be noted that given the on-sky position of K2-136, the ability to observe the system with JWST will be limited due to aperture position angle constraints. In addition, the very close ( $\sim 0.7$ ") stellar companion may

cause contamination of spectra from both instruments. This is a common issue for NIRISS since it is slit-less, but NIRSpec can usually isolate the primary target with its 1.6" square aperture. For K2-136 the companion star is well inside this aperture boundary and will likely create some contamination. The companion is significantly fainter than the host star (J magnitude of 14.1 vs 9.1), which should mitigate the impact to a degree. It should also be possible to reduce the companion M-star's spectral contamination effect in post-processing.

The most enticing feature of K2-136 is the young age of the system; it could be argued that despite the potential difficulty in observing the planets' atmospheres, the rewards outweigh the risks for the chance to better understand the atmospheres of very young, relatively small planets. Observations of this system could help us construct a picture of the environment and evolution of young, low-mass planets.

## 6. SUMMARY AND CONCLUSIONS

In this paper, we analyzed K2-136, a young system in the Hyades open cluster. The star is a K dwarf with  $M_*=0.742^{+0.039}_{-0.038}~{\rm M}_\odot$  and  $R_*=0.677\pm0.027~{\rm R}_\odot$ . It hosts three known, transiting planets with periods of 8.0, 17.3, 25.6 days, and radii of  $1.014 \pm 0.050 \,\mathrm{R}_{\oplus}$ ,  $3.00 \pm 0.13$  $R_{\oplus}$ , and  $1.565 \pm 0.077 R_{\oplus}$ . We gathered RV observations with the TNG HARPS-N spectrograph and ESPRESSO VLT spectrograph in order to measure the masses of the three planets. We find that K2-136c, a sub-Neptune and the middle planet of the system, has a mass of  $18.0^{+1.7}_{-1.6}$  ${\rm M}_{\oplus}$ . This corresponds to a density of  $3.69^{+0.67}_{-0.56}~{\rm g~cm^{-3}}$ (or  $0.67^{+0.12}_{-0.10} \rho_{\oplus}$ ). K2-136c is thus similar in mass to Neptune and Uranus but more than twice as dense as Neptune and nearly three times as dense as Uranus. K2-136c has a density consistent with an ocean world; a rocky, Earth-like core with solar metallicity atmosphere; and many other compositions. However, assuming an Earth-like rocky core and a H<sub>2</sub>-He envelope yields a H<sub>2</sub>-He mass fraction of  $\sim 5\%$ . K2-136b and K2-136d have RV signals too small to detect with our data set, but we have placed upper mass limits with 95% confidence of 4.3 and  $3.0 M_{\oplus}$ , respectively. Atmospheric characterization of K2-136c (or its siblings, if a firm mass measurement can be made), would be difficult but not necessarily unfeasible, and is the most practical way to narrow the compositional parameter space for these planets.

K2-136c is the smallest planet in an open cluster to have a mass measurement, and one of the youngest planets found to date smaller than Neptune. There are very few young planets with precise mass measurements, and even fewer as small as K2-136c. As a result, this system provides an important view of planet composition and evolution at ages that are relatively unexplored.

We are grateful to Eugene Chiang for useful feedback and advice regarding planetary formation and composition in this system.

A.W.M. is supported by the NSF Graduate Research Fellowship grant no. DGE 1752814. C.D.D. acknowledges support from the NASA K2 Guest Observer program through grant 80NSSC19K0099, the Hellman Family Faculty Fellowship, the Alfred P. Sloan Foundation (Grant FG-2019-11662), and the David & Lucile Packard Foundation (Grant 2019-69648).

This work has been partially supported by the National Aeronautics and Space Administration under grant No. NNX17AB59G.

The financial contribution from the agreement ASI-INAF n.2018-16-HH.0 is gratefully acknowledged.

Support for this work was provided by NASA through grants number HST-GO-15090.001-A and HST-GO-15091.001-A from the Space Telescope Science Institute, which is operated by AURA, Inc., under NASA contract NAS 5-26555.

This paper includes data collected by the *Kepler* mission. Funding for the *Kepler* mission was provided by the NASA Science Mission directorate.

Based on observations made with the Italian Telescopio Nazionale Galileo (TNG) operated by the Fundación Galileo Galilei (FGG) of the Istituto Nazionale di Astrofisica (INAF) at the Observatorio del Roque de los Muchachos (La Palma, Canary Islands, Spain).

LBo, GPi, IPa, VNa, and GLa acknowledge the funding support from Italian Space Agency (ASI) regulated by "Accordo ASI-INAF n. 2013-016-R.0 del 9 luglio 2013 e integrazione del 9 luglio 2015 CHEOPS Fasi A/B/C".

FL gratefully acknowledges a scholarship from the Fondation Zděnek et Michaela Bakala.

A.Mo. acknowledges support from the senior Kavli Institute Fellowships.

Some of the data presented in this paper was obtained from the Mikulski Archive for Space Telescopes (MAST). STScI is operated by the Association of Universities for Research in Astronomy, Inc., under NASA contract NAS5–26555. Support for MAST for non–HST data is provided by the NASA Office of Space Science via grant NNX13AC07G and by other grants and contracts.

This work has made use of data from the European Space Agency (ESA) mission Gaia (https://www.cosmos.esa.int/gaia), processed by the Gaia Data Processing and Analysis Consortium (DPAC, https://www.cosmos.esa.int/web/gaia/dpac/consortium). Funding for the DPAC has been provided by national institutions, in particular the institutions participating in the Gaia Multilateral Agreement.

This paper includes data collected with the TESS mission, obtained from the MAST data archive at the Space Telescope Science Institute (STScI). Funding for the TESS mission is provided by the NASA Explorer Program. STScI is operated by the Association of Universities for Research in Astronomy, Inc., under NASA contract NAS 5–26555.

Facilities: Kepler, TESS, Gaia, HST, VLT, TNG, XMM-Newton, NASA Exoplanet Archive, ADS, MAST Software: ARESv2 (Sousa et al. 2015), ATLAS (Kurucz 1993), BATMAN (Kreidberg 2015), isochrones (Morton 2015), JET (Fortenbach & Dressing 2020), lightkurve (Barentsen et al. 2019), MOOG (Sneden 1973), MultiNest (Feroz et al. 2009, 2013), RadVel (Fulton et al. 2018), SPOCK (Tamayo et al. 2020)

## REFERENCES

Aigrain, S., Llama, J., Ceillier, T., et al. 2015, MNRAS, 450, 3211 Babusiaux, C., Fabricius, C., Khanna, S., et al. 2022, arXiv e-prints, arXiv:2206.05989

- Bailer-Jones, C. A. L., Rybizki, J., Fouesneau, M., Demleitner, M., & Andrae, R. 2021, AJ, 161, 147
- Balucinska-Church, M., & McCammon, D. 1992, ApJ, 400, 699 Baraffe, I., Homeier, D., Allard, F., & Chabrier, G. 2015, A&A, 577, A42
- Barentsen, G., Hedges, C., Vinícius, Z., et al. 2019, KeplerGO/lightkurve: Lightkurve v1.0b29, doi:10.5281/zenodo.2565212
- Barnes, J. R., Collier Cameron, A., Donati, J. F., et al. 2005, MNRAS, 357, L1
- Barragán, O., Aigrain, S., Kubyshkina, D., et al. 2019, MNRAS, 490, 698
- Barragán, O., Armstrong, D. J., Gandolfi, D., et al. 2022, MNRAS, 514, 1606
- Batalha, N. E., & Line, M. R. 2017, AJ, 153, 151
- Benatti, S., Damasso, M., Borsa, F., et al. 2021, A&A, 650, A66 Benneke, B., Knutson, H. A., Lothringer, J., et al. 2019a, Nature Astronomy, 3, 813
- Astronomy, 3, 813
  Benneke, B., Wong, I., Piaulet, C., et al. 2019b, ApJ, 887, L14
  Borucki, W., Koch, D., Basri, G., et al. 2008, in IAU Symposium,
  Vol. 249, Exoplanets: Detection, Formation and Dynamics, ed.
  Y.-S. Sun, S. Ferraz-Mello, & J.-L. Zhou, 17–24
- Brandt, T. D., & Huang, C. X. 2015, ApJ, 807, 58
- Buchhave, L. A., Latham, D. W., Johansen, A., et al. 2012, Nature, 486, 375
- Burrows, A., Marley, M., Hubbard, W. B., et al. 1997, ApJ, 491,  $856\,$
- Burt, J. A., Nielsen, L. D., Quinn, S. N., et al. 2020, AJ, 160, 153
  Choi, J., Dotter, A., Conroy, C., et al. 2016, ApJ, 823, 102
  Ciardi, D. R., Beichman, C. A., Horch, E. P., & Howell, S. B. 2015, ApJ, 805, 16
- Ciardi, D. R., Crossfield, I. J. M., Feinstein, A. D., et al. 2018, AJ, 155, 10
- Collier Cameron, A., Mortier, A., Phillips, D., et al. 2019, MNRAS, 487, 1082
- Cosentino, R., Lovis, C., Pepe, F., et al. 2012, in Society of Photo-Optical Instrumentation Engineers (SPIE) Conference Series, Vol. 8446, Ground-based and Airborne Instrumentation for Astronomy IV, 84461V
- Cosentino, R., Lovis, C., Pepe, F., et al. 2014, in Society of Photo-Optical Instrumentation Engineers (SPIE) Conference Series, Vol. 9147, Ground-based and Airborne Instrumentation for Astronomy V, 91478C
- Cunha, D., Figueira, P., Santos, N. C., Lovis, C., & Boué, G. 2013, A&A, 550, A75
- Cutri, R. M., Skrutskie, M. F., van Dyk, S., et al. 2003, VizieR Online Data Catalog, 2246
- Demangeon, O. D. S., Zapatero Osorio, M. R., Alibert, Y., et al. 2021, A&A, 653, A41
- Desidera, S., Damasso, M., Gratton, R., et al. 2022, arXiv e-prints, arXiv:2210.07933
- Dotter, A. 2016, ApJS, 222, 8
- Dotter, A., Chaboyer, B., Jevremović, D., et al. 2008, ApJS, 178, 89
- Douglas, S. T., Curtis, J. L., Agüeros, M. A., et al. 2019, ApJ,  $879,\,100$
- Eastman, J., Gaudi, B. S., & Agol, E. 2013, Publications of the Astronomical Society of the Pacific, 125, 83
- Fernandez Fernandez, J., & Wheatley, P. J. 2021, arXiv e-prints, arXiv:2110.13754
- Feroz, F., Hobson, M. P., & Bridges, M. 2009, MNRAS, 398, 1601
  Feroz, F., Hobson, M. P., Cameron, E., & Pettitt, A. N. 2013, ArXiv e-prints, arXiv:1306.2144
- Fortenbach, C. D., & Dressing, C. D. 2020, PASP, 132, 054501Fortney, J. J., Marley, M. S., & Barnes, J. W. 2007, ApJ, 659, 1661
- Foster, G., Poppenhaeger, K., Ilic, N., & Schwope, A. 2022, A&A, 661, A23
- Fulton, B. J., Petigura, E. A., Blunt, S., & Sinukoff, E. 2018, PASP, 130, 044504
- Fulton, B. J., Petigura, E. A., Howard, A. W., et al. 2017, AJ, 154, 109
- Gaia Collaboration, Brown, A. G. A., Vallenari, A., et al. 2020, arXiv e-prints, arXiv:2012.01533
- Gaia Collaboration, & Vallenari, A. 2022, in prep
- Gaia Collaboration, Prusti, T., de Bruijne, J. H. J., et al. 2016, A&A, 595, A1

- Gaia Collaboration, Smart, R. L., Sarro, L. M., et al. 2021, A&A, 649, A6
- Giles, H. A. C., Collier Cameron, A., & Haywood, R. D. 2017, MNRAS, 472, 1618
- Gossage, S., Conroy, C., Dotter, A., et al. 2018, ApJ, 863, 67 Green, J. C., Froning, C. S., Osterman, S., et al. 2012, ApJ, 744, 60
- Gregory, P. C. 2007, MNRAS, 381, 1607
- Hayward, T. L., Brandl, B., Pirger, B., et al. 2001, PASP, 113, 105
- Haywood, R. D. 2015, PhD thesis, University of St Andrews, doi:10.5281/zenodo.35161
- Howe, A. R., Burrows, A., & Verne, W. 2014, ApJ, 787, 173
  Jenkins, J. M., Twicken, J. D., McCauliff, S., et al. 2016, in Society of Photo-Optical Instrumentation Engineers (SPIE) Conference Series, Vol. 9913, Software and Cyberinfrastructure for Astronomy IV, ed. G. Chiozzi & J. C. Guzman, 99133E
- Jin, S., Mordasini, C., Parmentier, V., et al. 2014, ApJ, 795, 65
   Kass, R. E., & Raftery, A. E. 1995, Journal of the American Statistical Association, 90, 773
- Kempton, E. M. R., Bean, J. L., Louie, D. R., et al. 2018, PASP, 130, 114401
- Kipping, D. M. 2013, MNRAS, 435, 2152
- Kitchatinov, L. L., & Olemskoy, S. V. 2012, MNRAS, 423, 3344Klein, B., Donati, J.-F., Moutou, C., et al. 2021, MNRAS, 502, 188
- Kreidberg, L. 2015, PASP, 127, 1161
- Kurucz, R. 1993, ATLAS9 Stellar Atmosphere Programs and 2
   km/s grid. Kurucz CD-ROM No. 13. Cambridge, Mass.:
   Smithsonian Astrophysical Observatory, 1993., 13
- Kurucz, R. L. 1992, in IAU Symposium, Vol. 149, The Stellar Populations of Galaxies, ed. B. Barbuy & A. Renzini, 225
- Lienhard, F., Mortier, A., Buchhave, L., et al. 2022, MNRAS, 513, 5328
- Livingston, J. H., Dai, F., Hirano, T., et al. 2018, AJ, 155, 115
  Lopez, E. D., & Fortney, J. J. 2013, ApJ, 776, 2
  —. 2014, ApJ, 792, 1
- Lopez, E. D., Fortney, J. J., & Miller, N. 2012, ApJ, 761, 59 Mamajek, E. E., & Bell, C. P. M. 2014, MNRAS, 445, 2169 Mandel, K., & Agol, E. 2002, ApJ, 580, L171
- Mann, A. W., Gaidos, E., Mace, G. N., et al. 2016, ApJ, 818, 46
  Mann, A. W., Vanderburg, A., Rizzuto, A. C., et al. 2018, AJ, 155, 4
- Martin, D. C., Fanson, J., Schiminovich, D., et al. 2005, ApJ, 619, L1
- Martín, E. L., Lodieu, N., Pavlenko, Y., & Béjar, V. J. S. 2018, ApJ, 856, 40
- Masuda, K., & Tamayo, D. 2020, AJ, 160, 224
- Mayo, A. W., Rajpaul, V. M., Buchhave, L. A., et al. 2019, AJ, 158, 165
- Mazeh, T., Holczer, T., & Faigler, S. 2016, A&A, 589, A75
   Mortier, A., Santos, N. C., Sousa, S. G., et al. 2013, A&A, 557, A70
- Mortier, A., Sousa, S. G., Adibekyan, V. Z., Brandão, I. M., & Santos, N. C. 2014, A&A, 572, A95
- Morton, T. D. 2015, isochrones: Stellar model grid package, Astrophysics Source Code Library, ascl:1503.010
- Mousis, O., Deleuil, M., Aguichine, A., et al. 2020, ApJ, 896, L22 NASA Exoplanet Science Institute. 2020, Planetary Systems Table, doi:10.26133/NEA12
- Pepe, F., Cristiani, S., Rebolo, R., et al. 2021, A&A, 645, A96
  Perryman, M. A. C., Brown, A. G. A., Lebreton, Y., et al. 1998, A&A, 331, 81
- Predehl, P., & Schmitt, J. H. M. M. 1995, A&A, 293
- Press, W. H., Teukolsky, S. A., Vetterling, W. T., & Flannery, B. P. 1992, Numerical recipes in FORTRAN. The art of scientific computing
- Queloz, D., Henry, G. W., Sivan, J. P., et al. 2001, A&A, 379, 279
  Rajpaul, V., Aigrain, S., Osborne, M. A., Reece, S., & Roberts, S. 2015, MNRAS, 452, 2269
- Raymond, S. N., & Morbidelli, A. 2020, arXiv e-prints, arXiv:2002.05756
- Rayner, J. T., Onaka, P. M., Cushing, M. C., & Vacca, W. D.
  2004, in Society of Photo-Optical Instrumentation Engineers (SPIE) Conference Series, Vol. 5492, Ground-based
  Instrumentation for Astronomy, ed. A. F. M. Moorwood & M. Iye, 1498–1509

- Rayner, J. T., Toomey, D. W., Onaka, P. M., et al. 2003, PASP, 115, 362
- Richey-Yowell, T., Shkolnik, E. L., Schneider, A. C., et al. 2019, ApJ, 872, 17
- Ricker, G. R., Winn, J. N., Vanderspek, R., et al. 2015, Journal of Astronomical Telescopes, Instruments, and Systems, 1, 014003Rigby, J., Perrin, M., McElwain, M., et al. 2022, arXiv e-prints,

arXiv:2207.05632

- Santos, N. C., Mortier, A., Faria, J. P., et al. 2014, A&A, 566, A35
- Sanz-Forcada, J., Micela, G., Ribas, I., et al. 2011, A&A, 532, A6Scargle, J. D. 1982, ApJ, 263, 835
- Schmitt, J. R., Agol, E., Deck, K. M., et al. 2014, ApJ, 795, 167
  Seager, S., Kuchner, M., Hier-Majumder, C. A., & Militzer, B. 2007, ApJ, 669, 1279
- Seager, S., & Mallén-Ornelas, G. 2003, ApJ, 585, 1038
- Skrutskie, M. F., Cutri, R. M., Stiening, R., et al. 2006, AJ, 131, 1163
- Sneden, C. A. 1973, PhD thesis, THE UNIVERSITY OF TEXAS AT AUSTIN.
- Sousa, S. G. 2014, ARES + MOOG: A Practical Overview of an Equivalent Width (EW) Method to Derive Stellar Parameters, ed. E. Niemczura, B. Smalley, & W. Pych, 297–310
- Sousa, S. G., Santos, N. C., Israelian, G., et al. 2011, A&A, 526, A99+
- Sousa, S. G., Santos, N. C., Mortier, A., et al. 2015, A&A, 576, A94
- Sozzetti, A., Torres, G., Charbonneau, D., et al. 2007, ApJ, 664, 1190
- Stefansson, G., Mahadevan, S., Maney, M., et al. 2020, arXiv e-prints, arXiv:2007.12766

Sun, L., Ioannidis, P., Gu, S., et al. 2019, A&A, 624, A15 Tamayo, D., Cranmer, M., Hadden, S., et al. 2020, Proceedings of

- the National Academy of Science, 117, 18194 Tayar, J., Claytor, Z. R., Huber, D., & van Saders, J. 2020, arXiv e-prints, arXiv:2012.07957
- Taylor, B. J. 2006, AJ, 132, 2453
- Torres, G. 1999, PASP, 111, 169
- Torres, G., Fischer, D. A., Sozzetti, A., et al. 2012, ApJ, 757, 161
  Tsantaki, M., Sousa, S. G., Adibekyan, V. Z., et al. 2013, A&A, 555, A150
- Van Eylen, V., Agentoft, C., Lundkvist, M. S., et al. 2018, MNRAS, 479, 4786
- Vanderburg, A., & Johnson, J. A. 2014, PASP, 126, 948
- Vanderburg, A., Latham, D. W., Buchhave, L. A., et al. 2016, ApJS, 222, 14
- Vanderburg, A., Huang, C. X., Rodriguez, J. E., et al. 2019, ApJ, 881, L19
- Vogt, S. S., Allen, S. L., Bigelow, B. C., et al. 1994, in
- Proc. SPIE, Vol. 2198, Instrumentation in Astronomy VIII, ed. D. L. Crawford & E. R. Craine, 362
- Wolfgang, A., Rogers, L. A., & Ford, E. B. 2016, ApJ, 825, 19
  Wright, E. L., Eisenhardt, P. R. M., Mainzer, A. K., et al. 2010, AJ, 140, 1868
- Wright, N. J., Newton, E. R., Williams, P. K. G., Drake, J. J., & Yadav, R. K. 2018, MNRAS, 479, 2351
- Xie, J.-W. 2014, ApJS, 210, 25
- Zacharias, N., Finch, C. T., Girard, T. M., et al. 2013, AJ, 145, 44 Zechmeister, M., & Kürster, M. 2009, A&A, 496, 577
- Zeng, L., & Sasselov, D. 2013, PASP, 125, 227
- Zeng, L., Sasselov, D. D., & Jacobsen, S. B. 2016, ApJ, 819, 127