

Supporting information

Ultra-low charge transfer resistance carbons by one-pot hydrothermal method for glucose sensing

Botao Hu¹, Jen-Tsai Liu^{1*}, Chingjung Chen^{2*}, Zhan Zhao^{2,3}, Shwu Jen Chang⁴ and Pei-Leun Kang⁵

* Corresponding author (email: jtliu@ucas.ac.cn (Liu J); cjchen@ucas.ac.cn (Chen C))

¹ College of Materials Science and Opti-Electronic Technology, University of Chinese Academy of Sciences, Beijing China

² School of Electronic, Electrical and Communication Engineering, University of Chinese Academy of Sciences, Beijing China

³ State Key Lab of Transducer Technology, Institute of Electronics, Chinese Academy of Sciences, Beijing China

⁴ Department of Electric Engineering, I-Shou University, Kaohsiung

⁵ Cardiovascular Surgery, Department of Surgery, Kaohsiung Veterans General Hospital, Kaohsiung

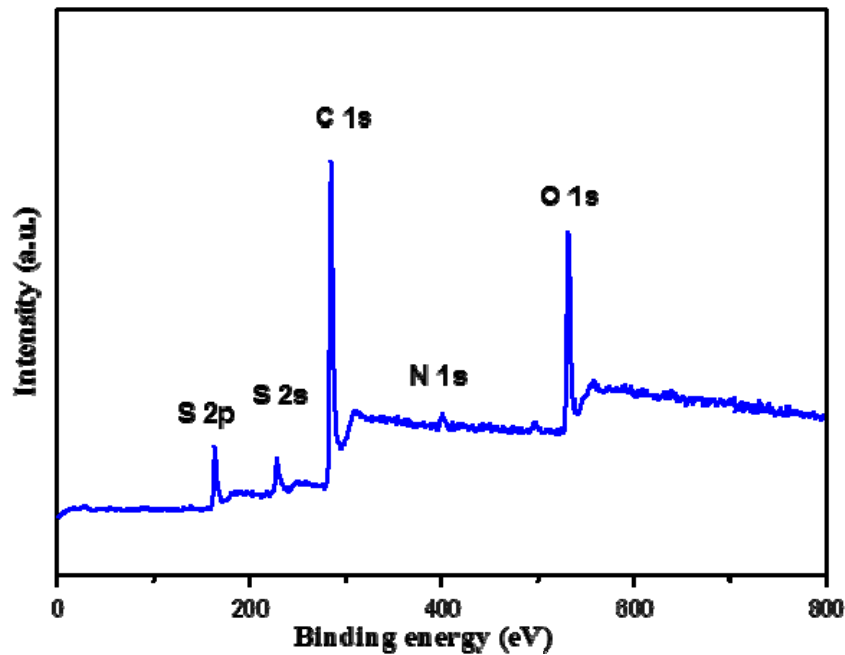


Figure S1 XPS spectrum survey scan of NS-C.

The high-resolution XPS spectrum is analyzed by program XPSPEAK. The high-resolution of N and S species doped in NS-C were measured 15 scans.